

RFP DOCUMENT NO. MPCB/JD(APC)/MMV/2021-22

Request for Proposal Document

For

SUPPLY, INSTALLATION AND COMMISSIONING
AND
OPERATION & MAINTENANCE SERVICES
OF
MOBILE CONTINUOUS AMBIENT AIR QUALITY MONITORING VAN (MCAAQMV)

For

Maharashtra Pollution Control Board



MAHARASHTRA POLLUTION CONTROL BOARD

Kalpataru Point, 3rd floor, Opp. Cine Planet Cinema, Sion Circle, Sion (E), Mumbai –400022

Tel: 24010437/24020781/24014701, Fax: 24044533 / 24023515 Website: http://www.mpcb.gov.in, E-mail: jdair@mpcb.gov.in,

INDEX

Chapter	Content	Page No
1	E- Tender- Invitation of Bids	10
2	Instructions to Bidders	15
3	Scope of Work	39
4	Schedule of Requirement	42
5	Form of Technical Bid	56
7	Form of Financial Bid	81
8	General Condition of Contract	90
9	Special Condition of Contract	111

Maharashtra Pollution Control Board

Kalpataru Point, $3^{\text{rd}}\&4^{\text{th}}$ Floor, Sion-Matunga Scheme Road No.8,

Opp. Sion Circle. Sion (East), Mumbai - 400 022

Website: http://mpcb.gov.in

Tender Notice

1) Tender Notice Details

Tender Reference no.	MPCB/JD(APC)/MMV/2021			
Name of Work / Item	Supply, installation and commissioning And Operation & maintenance services of Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMVV)- 15 Nos.			
Cost of blank tender document & Mode of Payment Rs. 20,000/- (Rupees Twenty thousand Only) (Non-Refundable) to be paid through Online Payment Modi.e. Net Banking only, during Tender Document Dow Stage.				
Rs. 65 lakh (Rupees sixty five lakhs only) by guarantee as per clause number 5.1 for Su Installation, Commissioning and Providing O & M Se of MCAAQMV to be installed in the State of Maharas (15 Nos).				
Date ,Time and Place of Pre Bid Meeting	24/08/2021 11:00 AM MPCB Conference Hall, Kalpataru Point, 4 th Floor, Sion, Matunga Scheme Road No.8, Opp. Sion Circle. Sion (East), Mumbai - 400 022 or through Video conferencing in view of COVID 19 lock down.			
Venue of online opening of e-tender MPCB Conference Hall, Kalpataru Point, 4 th Floor, Matunga Scheme Road No.8,Opp. Sion Circle. (East), Mumbai - 400 022				
Address for Communication	Member Secretary MPC Board, Kalpataru Point, 4 th Floor, Sion Matunga Scheme Road No.8,Opp. Sion Circle. Sion (East), Mumbai - 400 022			
Contact Telephone & Fax Numbers	022-24020781 /24010437 Fax : 022-24023516 Email- <u>jdair@mpcb.gov.in</u> , <u>airpams@mpcb.gov.in</u>			
e-Tendering Helpline Support:	24 X 7 Help Desk Toll Free No.1800 3070 2232 Mobile No. 7878007972, 7878007973, 7878007974.			

2) e-TENDER TIME SCHEDULE

Please Note: All bid related activities (Process) like Tender Document Download, Bid Preparation, and Bid Submission will be governed by the time schedule given under Key Dates below:

Sr. No.	Activity	Performed by	Start		Expiry	
			Date	Time	Date	Time (hrs.)
1	Release of E-tender	Department	17/08/2021	11:00	17/08/2021	17:00
2	E-tender Download		17/08/2021	17:01	04/09/2021	17:00
3	Clarification Start Date	Bidders	17/08/2021 17:01 Hrs			
4	Clarification End Date		23/08/2021 17:00 Hrs			
5	Pre-Bid Meeting	Department and Bidders	2	4/08/20	21 11:00 AM	
6	Bid Submission start Date	Bidders	24/08/2021	11:01	13/09/2021	17:00
7	Envelope Opening Date (Technical Bid)	Department	20/09/2021	11:00	21/09/2021	17:00
9	Envelope Opening Date (Price Bid)	Department		To be anı	nounce later	

^{*}Dates mentioned here, are scheduled dates for Bid Opening Activities. Any changes in dates of opening of technical and commercial bids shall be notified in 'Press Notice / Corrigendum' section on the e-Tendering sub portal of the department before opening of the same.

Note: MPCB reserve the Right to alter / change above schedule under unavoidable circumstances and such changes will be displayed at MPCB web site: www.mpcb.gov.in

3. INSTRUCTIONSTO BIDDERS

3.1 INSTRUCTIONS TO BIDDERS FOR e-Tendering

GENERAL INSTRUCTIONS:

The bidders are requested to familiarize themselves with the use of the e-Tendering portal of Government of Maharashtra well in advance

To view- Tender Notice, Detailed Time Schedule, Tender Document and BoQ for this Tender and subsequently purchase the Tender Document and its supporting documents, kindly visit following e-Tendering website of **Government of Maharashtra** www.mahatenders.gov.in

All bidders interested in participating in the online e-Tendering process are required to procure Class II or Class III Digital e-Token having 2 certificates inside it, one for Signing/Verification purpose and another for Encryption/Decryption purpose. The tender should be prepared & submitted online using individual's Digital e-Token.

The Contractors participating first time for e-Tenders on Maha e-tendering portal will have to complete the Online Registration Process for the e-Tendering portal. A link for enrolment for new bidders are as follows

https://mahatenders.gov.in/nicgep/app;jsessionid=CA1444774BB4186D0E04B4178D5CA501.mhgeps2?page=BiddersManualKit&service=page

Empanelment: The Contractors interested in participating in the Tenders of Maharashtra Pollution Control Board processed using the Electronic Tendering System shall be required to enrol on the Electronic Tendering System to obtain Login ID and password.

The Contractors may obtain the necessary information on the process of enrolment either from Helpdesk support team or enrolled directly on Web site www.mahatenders.gov.in.

e-Tendering Tool Kit for Bidders

(detailed Help documents, designed for bidders) has been provided on Mahaetender website

https://mahatenders.gov.in/nicgep/app;jsessionid=CA1444774BB4186D0E04B4178D5CA501.mhgeps2?page=BiddersManualKit&service=page order to guide them through different stages involved during e-Tendering such as online procedure for Tender Document Purchase, Bid Preparation, Bid Submission.

Bidders will have to pay cost of Tender Document through online modes of payment by **Net Banking only,** during **Tender Document Download stage**. This payment will not be accepted by the department through any offline modes such as Cash, Cheque or Demand Draft.

Similarly, Bidders will have to pay Earnest Money Deposit by bank guarantee as per clause number 5.1. This payment will not be accepted by the department through any offline modes such as Cash, Cheque or Demand Draft.

For any assistance on the use of Electronic Tendering System, the Users may call the below numbers:-

24 X 7 Help Desk Toll Free No.1800 3070 2232 Mobile No. 7878007972, 7878007973, 7878007974.

For a bidder, online bidding process consists of following 3 stages:

- 1. Online Tender Document Purchase and Download
- 2. Online Bid Preparation
- 3. Online Bid Submission

All of 3 stages are mandatory in order for bidders to successfully complete Online Bidding Process.

TENDER DOCUMENT PURCHASE AND DOWNLOAD:

The tender document is uploaded / released on Mahaetenders website

<u>www.mahatenders.gov.in</u> Tender document and supporting documents may be purchased and downloaded from following link as above by making payment through **Online Payment Modes i.e. Net Banking Only.**

If for any reason a bidder fails to make this payment through online modes, system won't allow the bidder proceed further for next stage resulting in his/her elimination from Online Bidding Process.

This payment will not be accepted by the department through any offline modes such as Cash, Cheque or Demand Draft.

Subsequently, bid has to be prepared and submitted online ONLY as per the schedule.

The Tender form will be available online only. Tender forms will not be sold / issued manually. The bidders are required to download the tender document within the pre-scribed date & time mentioned in online tender schedule. After expiry of the date and time for tender document download, Department / Corporation will not be responsible for any such failure on account of bidders for not downloading the document within the schedule even though they have paid the cost of the tender to the Department / Corporation. In such case the cost of the tender paid by the bidders will not be refunded.

1 PREPARATION & SUBMISSION OF BIDS

Bids shall have to be prepared and subsequently submitted online only. Bids not submitted online will not be entertained.

2 Online Bid Preparation Price BID

All commercial offers must be prepared online as per given BoQ format (An online form will be provided for this purpose in Online Price Bid Envelope during **Online Bid Preparation** stage).

Online Bid Submission

In this stage, bidders who have successfully completed their Bid Preparation stage are required to submit the bid,

INSTRUCTION TO BIDDERS FOR ONLINE BID PREPARATION & SUBMISSION

Bidders will have to pay Earnest Money Deposit by bank guarantee as per clause number 5.1. This payment will not be accepted by the department through any offline modes such as Cash, Cheque or Demand Draft.

During the activity of **Bid Preparation**, bidders are required to scanning the documents and uploading those in the PDF format. This apart, bidders will have to quote commercial offer for the work / item, for which bids are invited, in an online form made available to them in Commercial Envelope. This activity of **Bid Preparation** should be completed within the pre-scribed schedule given for bid preparation.

After **Bid Preparation**, the bidders are required to complete **Bid Submission** activity within prescribed schedule without which the tender will not be submitted.

The date and time for online preparation followed by submission of envelopes shall strictly apply in all cases. The tenderers should ensure that their tender is prepared online before the expiry of the scheduled date and time and then submitted online before the expiry of the scheduled date and time. No delay on account of any cause will be entertained. Offers not submitted online will not be entertained.

If for any reason, any interested bidder fails to complete any of online stages during the complete tender cycle, department shall not be responsible for that and any grievance regarding that shall not be entertained.

Any amendment to the tender will be placed on sub portal of the Department, who have invited the bids, on Maha e-tendering portal. The tenderer will not be communicated separately regarding the amendment.

OPENING OF BIDS:

The bids that are submitted online successfully shall be opened online as per date and time given in detailed tender schedule (if possible), through e-Tendering procedure only in the presence of bidders (if possible). Bids shall be opened either in the presence of bidders or its duly authorized representatives. The bidder representatives who are present shall sign a register evidencing their attendance. Only one representative per applicant shall be permitted to be present at the time of opening the tender.

7). TECHNICAL BID

TECHNICAL BID ENVELOPE

This envelope shall be opened online as per the date and time given in detailed tender schedule (if possible), through e-Tendering procedure only,

The list of documents for Technical Envelope is as follows:

Sr. No.	List of Documents	Compulsory (C) / Additional (A)
1	Form of Questionnaire as per attachment I of volume I (Section III)	С
2	Certificate of O & M partner of the Bidder in India as per attachment 2 of volume I (Section III)	С
3	Form of letter of authority as per attachment 3 of volume I (Section III)	С
4	Form of certificate of supply of spares and consumables by manufacturer as per attachment 3A of volume I (Section III).	С
5	Form of Certificate of Country of Origin as per attachment 4 of Volume I(Section III).	С
6	Form of certificate of carrying out O & M of MCAAQMV by the O & M Partner in India as per attachment 5 in Volume I (Section III).	С
7	Form of Equipment List as per attachment 6 in volume I (Section III).	С
8	Form of manufactures list as per attachment 7 in volume I (Section III).	С
9	Proforma for financial capability for bidder as per attachment 8A in volume I (Section III).	С
10	Proforma for performance statement for manufacturer as per attachment 8B in Volume I (Section III).	С
11	Proforma for performance statement for Authorized Representative of the Manufacturer as per attachment 8C in Volume I (Section III).	С
12	Capability & experience of O & M Partner as per attachment 9 in Volume I (Section III).	С
13	Form for Pre-requisite for Installation of equipment as per attachment 11 in Volume I (Section III).	С
14	Deviation Schedule as per attachment 12 in Volume I (Section III).	С
15	Technical data sheet for supply and O & M as per Annexure I of Volume II.	С

Note: 1) C indicates compulsory documents to be uploaded in PDF format online.

- 2) All catalogs and other supporting documents for above items & other Terms of Conditions of technical bids shall also be submitted in hard copy at the time of technical bid opening.
- 3) Bidder has to upload all above documents online. If fails to upload, technical bid will be treated as non-responsive.

Price Bid ENVELOPE:

This envelope shall be opened online as per the date and time given in detailed tender schedule (if possible), through e-Tendering procedure only.

Sr. No.	List of Documents	Compulsory/ Additional (A)
1	Bid Form as per Attachment- 1 of financial bid (Volume I, Section IV)	С
2	Summary of Bid price as per Attachment – 2 (Section IV)	С
3	Bid price break up of equipment of foreign origin (CIF – price) as per Attachment – 3 (Section IV)	С
4.	Bid price breakup for O & M of MCAAQMV for five years as per Attachment -3 A (Section IV)	С

Note: 1) The Price bid documents should be uploaded in given BoQ format only and Online.

No documents should be submitted in hard copy

INVITATION FOR BIDS (IFB) BIDDING DOCUMENT

No. e-Tender: MPCB/JD(APC)/MMV/2021 Date: . .2021

PROJECT: Supply, installation and commissioning and Operation & maintenance services of Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV)

- 1. Maharashtra Pollution Control Board, invites bids in two Bidding system (Technocommercial bid and financial Bid through online from eligible bidders for Supply, Installation, Commissioning of Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV) for the State of Maharashtra- 15 No.(listed in Bid documents) and Operation & Maintenance of Continuous Ambient Air Quality Monitoring Analysers (CAAQMA) fitted within mobile vehicle, at various locations as listed and related services as specified in the bid document. The operation and maintenance of Mobile vehicle would also be responsibility of bidder. Vendor shall supply total Fifteen (15) no. of fully assembled Mobile CAAQMV and same shall be used for monitoring at the different locations. The Mobile CAAQMV shall consist of analysers, sample hoods, signal convertors, data loggers, printers, calibrators, sample handling Equipments, weather monitoring instruments, racks, special tools, calibration gas cylinders, zero air generators, multipoint calibrator, Petrol Generator set, air conditioners (roof-mounted, if required), and related service as specified in the bid document as a minimum.
- 2. This invitation for the Bid is open to eligible bidder who is a reputed manufacturer or authorized representative of the manufacturer, who on its own or along with his associate as O & M partner meets the qualifying Requirements stipulated hereunder for participation in the tender. The bidder shall furnish satisfactory evidence to establish that bidder meets the following qualifying requirements.
- 2.1 The bidder should have at least five years' experience in supply and satisfactory operation and maintenance of real time (Continuous) ambient air quality monitoring system (CAAQMS).
- 2.2 For all the items not manufactured by the Bidder i.e. Analysers, Monitors, Calibrators and Sensors, the bidders should be authorized by the manufacturers for these items as per the format "Form of letter of authorities" provided as Attachment 3 of Section III.
- 2.3 Bidder shall procure Mobile vans(vehicles) as per the specifications of the tender in the name of "Maharashtra Pollution Control Board" to be fitted with analysers.
- 2.3 Bidder or their authorized representative should have adequate financial capability to execute the contract and should be profitable for each of the past 3 years ending 31st March, 2021. Average turnover of the bidder for last three years should not be less than INR 60 Crs as per Attachment 8A of section III.
- 2.4 The bidder should furnish the information on all past supplies and satisfactory performance of CAAQMS analysers, in "Performance Statement" as per Attachment No. 8B of Section III and minimum five (5) nos. documentary evidences (client certificates in favours of bidder or manufacturers of equipment) in support of the satisfactory operation of CAAQMS and minimum two (2) documentary evidence for Mobile air quality monitoring vans.

- 2.5 The bidder or its associates as an O &M partner in India, (any authorized agency in India) should have well trained O & M personnel on its regular rolls as per following details and on award of LOI bidder shall submit the name of Project Engineer (Grad. Engineer), Technicians (Diploma holder in electronics/ instrumentation) and Data Processor for central data management and CAAQM station respectively. Their resume, PF slip as a proof of their regular employment with the bidder. All personnel should be on pay roll of the O & M partner.
- 2.6 The O&M partner shall furnish an undertaking regarding carrying out satisfactory O &M of MCAAQMV covered in this document as per terms & conditions of the document on behalf of the bidder. This information is to be provided as per Attachment 5 & 9 of Section III.
 - 2.7 A complete set of bidding documents can be downloaded by any interested eligible bidder from the website of GoM www.mahatenders.in. The payment of Bid Document Fee should be made online which is non-refundable.
 - 2.8 This bidding takes simultaneous bidding procedure in two-part (envelope) bidding system. All the eligible and interested bidders are required to submit the Techno-commercial bid and Financial Bid simultaneously. Only the bidders whose Techno-commercial bid is found substantially responsive, will be notified by the Board of the date and place to participate in the public opening of the financial bid, in writing later.
 - 2.9 Eligible Bidders must submit their bids online for complete scope of work. Any bid submitted for incomplete scope shall be rejected out rightly.
 - 2.10 The Representative of Foreign Bidders in India are also permitted to purchase Tender Document on behalf of their principals by submitting a letter of authority (user login Id / Key's for submitting of EMD) from their principals and by depositing requisite cost of tender document.
 - 2.11 All the bids must be accompanied by bid security in accordance with the Instructions to Bidders in the bidding documents.
 - 2.12 All bids must be submitted on or before as per the e-Tender time scheduled. Any offer received after expiry of the time and date prescribed for receiving complete bid will not be entertained. Only the technical Bid will be opened in presence of the bidders or their representative, who choose to attend on the specified date and time at the office of MAHARASHTRA POLLUTION CONTROL BOARD (MPCB).
 - 2.13 Downloading of Bidding Documents will not be construed to mean that such bidders are automatically considered qualified.
 - 2.14 The bid must accompany bid security money as indicated above, failing which it will not be accepted online.
 - 2.15 MPCB will not be responsible for any cost(s) or expense(s) incurred by bidders in connection with the preparation or uploading/delivery of bids.
 - 2.16 The MPCB reserves the right to reject any or all the bids without assigning any reason whatsoever.
 - 2.17 In the event of date being declared as a closed holiday the date for submissions of bids and opening of bids will be the following working day at the appointed time.
 - 2.18 Interested eligible Bidders may obtain further information from Administrative Branch of MPCB for the bidding documents.

- 2.19 Description of works shall be as per Annexure I enclosed below.
- 2.20 The original and all copies of the bid (Without Financial Bid) shall be typed or written in indelible ink and shall be stamped & signed by authorized Person of the Bidder. The Bidder shall submit online whole technical bid (Without Financial Bid) document along with Technical Bid stamped & signed by authorized Person of the bidder.
- 2.21 The Financial Bid must be done only online on the website: www.mahatenders.in
- 2.22 The Successful bidder shall be signing the Contract Agreement with MPCB Head Office, Mumbai after submitting the required Performance Bank Guarantee.

ANNEXURE - I (For 01(One) MCAAQMV)

SI. No.	Name of the Vehicle instrument/ Equipment	Quantity (Nos.)	Cost of B.O.Q. (in Rs.)
1.	Automatic Ambient CO Analyzer	01	
2.	Automatic Ambient SO₂ Analyzer	01	
3.	Automatic Ambient NO-NO ₂ -NOx Analyser	01	
4.	Automatic Ambient O3 Analyser	01	
5.	PM ₁₀ Monitor	01	
6.	PM _{2.5} Monitor	01	
7.	BTX Analyzer	01	
8.	Multi-calibration systems for gaseous monitors comprising of gas supply/generation and automated calibration	01	
9.	Sensor Based Meteorological Instrumentation comprising Wind Direction, Wind Speed, Ambient Temperature, Relative Humidity, Solar Radiation and Rainfall mounted on telescoping crank up meteorological Mast.	1 Set	
10.	Computer system consisting of one PC along with Laser Printer and DAS at the monitoring Van and one PC with colour printer cum scanner at central office with peripherals and software for data acquisition / Data display Board /transfer and system integration, telephone, Modem.	1 Lot	
11.	Arrangements like Thermally Stable Housing (Body Built up) for installation of Continuous Ambient air quality Monitoring analysers with Sampling line, Internal fittings, Instruments racks, Electrical and Gas line Fittings, Tools (electrical and mechanical).	1 Lot	
12.	2 Ton capacity split Air conditioner	2 Units	
13.	Petrol Generator set-6.5 KVA	1 Unit	
14.	Stabilizer KVA	1 Unit	
15.	Vehicle model number TATA LPT 709Ex 2 or its equivalent, BS-VI variant along with vehicle frame (Chassis build up) air conditioned and thermally stable instrument cabin.	1 Unit	
16.	Annual operation & Maintenance of Continuous Air Quality Monitoring Analyser Systems along with Mobile Vehicle for five years		

Note: 1. Total quantity shall be 15 nos. of MCAAQMV.

2. List of the City / Locations where MCAAQMV will be parked as mentioned below.

MCAAQMV: (Total 15 Nos.)

	Regional Offices, Maharashtra Pollution Control Board
1	Regional Officer, Mumbai, Maharashtra Pollution Control Board, 1 st Floor, Kalpataru Point, Sion-East, Sion, Mumbai -400 022.
2	Regional Officer, Navi Mumbai, Maharashtra Pollution Control Board, Raigad Bhavan, 7 th Floor, CBD-Belapur, Navi Mumbai -400 614.
3	Regional Officer, Raigad , Maharashtra Pollution Control Board, Raigad Bhavan, 6 th Floor, CBD-Belapur, Navi Mumbai-400 614
4	Regional Officer, Nagpur, Maharashtra Pollution Control Board, Udyog Bhavan, 5 th Floor, Near Sales Tax Office, Civil Lines, Nagpur -440 001.
5	Regional Officer, Nashik, Maharashtra Pollution Control Board, Udyog Bhavan, 1st Floor, Trimbak Road, Near ITI, Satpur, Nashik -422 007.
6	Regional Officer, Thane, Maharashtra Pollution Control Board, Plot No. P-30, 5 th Floor, Office Complex Building, Near Mulund Check naka, Thane -400 604.
7	Regional Officer, Pune, Maharashtra Pollution Control Board, Jog Centre, 3 rd Floor, Mumbai-Pune Road, Wakdewadi, Shivaji Nagar, Pune -411 003.
8	Regional Officer, Aurangabad, Maharashtra Pollution Control Board, A-4/1, MIDC Area, Chikalthana, Near Seth Nandlal Dhoot Hospital, Jalna Road, Aurangabad -431 210.
9	Regional Officer, Kalyan, Maharashtra Pollution Control Board, Siddhivinayak Sankul, 3 rd & 4 th floor, Oak Baug, Station Road, Kalyan (West)-421 301.
10	Regional Officer, Chandrapur, Maharashtra Pollution Control Board, 1 st floor, Udyog Bhavan, Railway Station Road, Chandrapur -442 401.
11	Regional Officer, Amravati Maharashtra Pollution Control Board, 18/25, Ashirwad Building, Daffrin Hospital Road, Shrikrishna Peth, Amravati -444 601.
12	Regional Officer, Kolhapur, Maharashtra Pollution Control Board, Udyog Bhavan Building, Near Collectorate Office, Kolhapur -416002.

The details about remaining 3 nos. of MCAAQMV will be provided informed at later stage but they are in the state of Maharashtra only.

VOLUME 1

SECTION I (ITB)

INSTRUCTIONS TO BIDDERS

CONTENTS

1.	Definitions	16
2.	Introduction	17 to 21
3.	Bidding Documents	21 to 23
4.	Preparation and Submission of Bid	23 to 25
5.	Preparation of Techno-commercial Bid	25 to 28
6.	Preparation of Financial Bid	28 to 30
7.	Submission of Bid	30 to 32
8.	Opening and Evaluation of Techno-commercial Bid	33 to 36
9.	Notification of Successful Techno-commercial Bid	36
10.	Opening of Financial Bid	36
11.	Examination of Financial Bid	36 to 37
12.	Evaluation and Comparison of Financial Bid	37 to 39
13.	Award of Contract	39 to 40
14.	Performance Security	40
15.	Expense of Bid	40
16.	Responsibility for information supplied	40

Important: Bidders are expected to examine the Bidding Documents carefully and are deemed to have received and read all documents. It shall be the responsibility of the Bidder to request copied of any missing documents. Failures to do so will be at the Bidder's risk.

INSTRUCTION TO BIDDERS

1.0 DEFINITIONS

The terms used in this bidding document shall have the meaning defined hereunder:

- 1.1 "The Project" or "The Works" means Supply, Installation, Commissioning of MCAAQMV to be handed over to MPCB- 15 Nos. and Operation & Maintenance of this Continuous Air Quality Monitoring Analyser System along with Mobile Vehicle at the pre-defined city/ location.
- 1.2 "The Board" means the MAHARASHTRA POLLUTION CONTROL BOARD, having its Head office at Mumbai, India and shall include any person or persons authorized by the Board. The Board is also executing agency of the Project. "The **Owner**" means the Board.
- 1.3 "The Bid" means the offer or proposal of the Bidder to be submitted for the works in accordance with the stipulations set forth in this Bidding Documents.
- 1.4 "The Techno-commercial Bid" means the Techno-commercial part of the Bid.
- 1.5 "The Financial Bid" means the financial part of the Bid.
- **1.6** "The Bidder" means either the manufacturer of the Equipment or his authorized Representative, who submits the Bid for the Works.
- 1.7 "The Authorized representative" means the bidder who has enclosed the manufacturer's authorization as per the format "Form of letter of authorities" provided as Attachment 3 of Section III.
- **1.8** "The Contractor" or "The Contractor" means the Bidder, whose Bid for the Works has been accepted by the Board and includes his personal representatives, successors and authorized assignees.
- **1.9** "The Manufacturers" means the firms, which produces the equipment to be furnished by the Contractor under the Contract with the Board.
- **1.10** "The Bidding Documents" mean all the documents in Volume I and II in the bidding documents annexed thereto.
- 1.11 "The Contract" means the written agreement to be concluded between the Board and the Contractor and includes terms and conditions stipulated on the Bidding Documents and any other descriptions annexed there to which form an integral part of the agreement to be provided by the Board.
- **1.12** "The Equipment" means all kind of materials, machinery, components, apparatus, articles and instruments for the Project to be provided by the Contractor to the Board under the Contract.

- 1.13 "The Specifications" means the specifications of the Works to be performed by the Contractor in conformity with those specified in the Technical Specifications of Volume II and all other related documents in the Bidding Documents, and modifications thereof or additions thereto as may from time to time be made and approved in writing by the Board in case prior to the Contract and agreed upon by both the Board and the Contractor after the Contract.
- 1.14 "S/W" means the Scope of Works in Section II of this Volume.
- 1.15 "The Sites" means MCAAQMV at the defined city/ location.
- **1.16** "The Contract Price" means the price payable to the contractor under the contract for the full and proper performance of its contractual obligations.
- 1.17 "Analyser System" means complete set of equipment / instruments / accessories / attachments / calibration gases / calibration systems / electronics / logistic etc required to sample / monitor continuous ambient air quality through various approved analysers along with data acquisition system and computer with peripherals.

2.0 INTRODUCTION

2.1 The MAHARASHTRA POLLUTION CONTROL BOARD intends to invite bids from eligible bidders for Supply, installation and commissioning and Operation & maintenance services of Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV) fitted with Continuous Air Quality Monitoring Analyser System along with Mobile Vehicle at specified city / locations wise.

2.2 Scope of Works

The description of Scope of Works is set forth in Section II of this Volume 1.

2.3 Size of Bid

The whole bid is for single composite package as detailed at Section II i.e. scope of work.

2.4 Eligible Equipment and conformity to the bidding documents

- (1) All countries are the eligible source countries for goods and services to be supplied under this contract.
- (2) For the purpose of this clause "origin" means the place where the equipment or component parts thereof are grown, or produced. Equipment are produced when, through manufacturing, processing or substantial and major assembling of components, a commercially recognized product results that is substantially different in basic characteristics or in purpose or utility from its components.

- (3) The Bidder shall furnish the Certificate of Country of Origin (duly authenticated by competent authority of that country) of each Equipment (as per Attachment 4 to Section III) in these instructions, as the documentary evidence of the eligibility of the Equipment.
- (4) The origin of equipment may be distinct from the nationality of the bidders.
- (5) Conformity of the Bidding documents may be in the form of literature, drawings, and data, and the Bidder shall also furnish:
- a) A detailed description of equipment, essential technical and performance characteristics.
- b) A list giving full particulars, including available sources of all spares (whether mandatory or recommended) and their prices, special tools etc., necessary for the proper and continued functioning/ maintenance of the equipment on long term basis.
- c) An inventory of the spare parts for each equipment available with the O&M partner in India mentioning the ones not available in India and have to be imported in case necessary after the expiry of O&M period.
- d) A clause-by-clause commentary of the Board's Technical Specifications demonstrating the equipment's substantial responsiveness of these specifications or a statement of deviations of exceptions to the provisions of Technical Specifications.

The above stated requirements are a minimum and the Board reserves the right to request any additional information concerning the Bid Proposal in response to this Invitation of Bids.

2.5 Qualifying Requirements of Bidders

This invitation for the Bid is open to eligible bidder who is a reputed manufacturer or authorized representative of the manufacturer, who on its own or along with his associate as O&M partner meets the Qualifying Requirements stipulated hereunder for participation in the tender. The bidder shall furnish satisfactory evidence to establish that bidder meets the following qualifying requirements.

2.5.1 The bidder should be a manufacturer or an authorized agent listed in the scope of work and must have supplied, manufactured, installed, commissioned minimum Two (02) nos. of mobile ambient air quality monitoring vans in their existing tenure and must have commissioned minimum 05 nos. of CAAQMS stations with 08 parameters in the last three years and should be in satisfactory operation

- 2.5.2 For all the items not manufactured by the Bidder i.e. Analysers, Monitors, Calibrators and Sensors, the bidders should be authorized by the manufacturers for these items as per the format "Form of letter of authorities" provided as Attachment 3 of Section III.
- 2.5.3 Bidder or their associate as O&M partner should have adequate financial capability to execute the contract as per Attachment 8A of section III.
- 2.5.4 Bids of bidders quoting as authorized representative of a **manufacturer**, **who meets the above requirements** in full, can also be considered, provided:
 - the manufacturer furnishes a legally enforceable authorization certificate in the prescribed format Attachment-3 Section-III, assuming full guarantee and O & M obligations as per GCC and SCC, for the goods offered; and
 - (ii) The bidder should be a manufacturer or authorized agency as listed in the scope of work who must have manufactured, supplied, tested, commissioned/built and provided O & M to minimum Two (02) nos. similar Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV) in their existing tenure and should have supplied, commissioned minimum Five (05) nos. of Continuous Ambient Air Quality Monitoring Stations (CAAQMS); for monitoring Eight (8) number of notified parameters as per AQ Standards 2009 in the last three years and which should be in satisfactory operation as on date of bid opening.
- 2.5.5 The bidder should furnish the information on all past supplied and satisfactory performance for both 2.5.1 and 2.5.4 (ii) above, in "Performance Statement" as per Attachment No. 8B & 8C respectively of Section III and minimum two (2) nos. documentary evidences (client certificates in favour of bidder or manufacturers of equipment) in support of the satisfactory operation of similar mobile air monitoring stations, which is in use for last two (2) years and to provide documentary evidence of five(5 no.) of CAAQMS operated satisfactorily.
- 2.5.6The bidder or their associates with an O&M partner in India, (any authorized agency in India) should have well trained O&M personnel on its regular rolls as per following details. To establish this bidder should enclose the curriculum vitae of following persons with required experience. The bidder should submit the copy of the service bond agreement between employer (bidder) and employee (personal i.e. Project Manager, Technician and Data Processor) for duration mention in below table at the time of bid submission.

SI. No.	Responsibility	No. of Persons	Minimum Qualification	Experience	Service Bond Duration
1.	Project Manager	01	Graduate Engg./ M.Sc.	10 years	5 Years (min)
2.	Technician**	15	Diploma in Electronics/Instrumentat ion/Electrical	3 years	5 Years (min)
3	Data Processor*	01	Science Graduate	2 Years	5 Year (min)

^{*} To be stationed at MPCB-HQ. ** Stationed at each Mobile Van.

- 2.5.7 The O&M partner shall furnish an undertaking regarding carrying out satisfactory O & M of Continuous Air Quality Monitoring Analyser System and monitoring Vans covered in this document as per terms &conditions of the document on behalf of the bidder. This information is to be provided as per Attachment 5 & 9 of Section III.
- 2.5.8 The Bidder and their Principal firm have to give undertaking that they will continue the formal collaboration till the entire duration of O & M contract. The spares/consumables will be supplied by the Principal firm to representative firm till entire duration of O & M contract of mobile monitoring vans / CAAQMS.

2.6 Bidding Procedure

- (1) The Bidding will take two envelopes simultaneous Bidding procedure.
- (2) All bids shall be submitted simultaneously by the designated date and at the place specified in Sub-clause 7.2 in this instruction. The Technical Bid will be evaluated first and only the Bidders who's Technical Bids will have been found substantially responsive will be notified by the Board of the date and place to participate in the publicly opening of the Financial Bid in writing.
- (3) The envelop for Technical Bid shall consist of three (3) envelopes. The first envelope "A" will contain the Bid Security; the second envelope "B" will contain the qualification documents, and the third envelope "C" will contain the technical specifications pursuant to Clause 5 of this Instructions.
- (4) The Financial Bid documents must be pursuant to Clause 6 of these Instructions.
- (5) The bidder must quote for complete scope of work in package. In case the bidder does not quote for complete scope of work, the bid shall be rejected at Techno-commercial evaluation stage.

The bidder shall bear all costs associated with the preparation and delivery of its bid, and purchaser will in no case be responsible or liable for those costs.

3.0 BIDDING DOCUMENTS

3.1 Downloading of Documents

A complete set of bidding documents can be downloaded by any interested eligible bidder from the website http://maharashtra.etenders.in from 17/08/2021.

The payment of Bid Document shall be made in INR to MAHARASHTRA POLLUTION CONTROL BOARD, online only, which is non-refundable.

Bidding Documents are not transferable.

3.2 Confidentiality of Documents

All recipients of the Bidding Documents, regardless of whether the Bid is submitted or not, shall treat the details of the documents as private and confidential.

3.3 Check of the Bidding Documents

Upon receipt of the Bidding Documents, the Bidder shall check the number of pages and drawings and notify the Board of any missing or duplicate pages and drawings or of any figures or words, which may be indistinct or ambiguous.

No claim will be admitted as result of the Bidder's failure to comply with the foregoing. The address for the contact is specified in Sub-clause 3.5 of this Instruction.

3.4 Contents of Bidding Documents

(1) The Bidding Documents include:

<u>Volume I</u>

NOTICE: E-TENDER – INVITATION FOR BIDS

SECTIONI INSTRUCTION TO BIDDERS

SECTIONII SCOPE OF WORKS

SECTION III FORM OF TECHNO-COMMERCIAL BID

SECTIONIV FORM OFFINANCIAL BID

SECTION V GENERAL CONDITIONS OF CONTRACT

SECTION VI SPECIAL CONDITIONS OF CONTRACT

Volume II

Technical Specifications

(2) Bidders must acquaint themselves with all the Bidding Documents embodied in Volume I and Volume II. In order to familiarize with the Works, the Bidders should ascertain all particulars regarding the location and site conditions at their own expenses. No plea attributed to lack of information or insufficient information will be entertained at any time.

The Board shall reserve the right and privilege to settle the affairs in case any doubt may occur concerning the Bidding Documents.

3.5 Clarification of Bidding Documents

If a prospective Bidder has any doubt as to the meaning of any part of the Bidding Documents, bidder may notify the Board for supplementary information and explanation in writing or facsimile in compliance with Form of Questionnaire of Attachment 1 in Section III at the following address before Pre- bid meeting.

Member Secretary
Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, Sion (East), Mumbai – 400 022, *E-mail: idair@mpcb.gov.in*,

3.6 Amendment of Bidding Documents

- (1) At any time prior to the deadline for submission of the Bid, the Board, for any reason, whether at its own initiative or in response to a clarification requested by a prospective Bidder, may modify the Bidding Documents by amendment.
- (2) All prospective Bidders who have received/downloaded the Bidding Documents will be notified of the amendment in writing at the address contained in their letter of request for issue of bidding documents and will be binding on them. The MPC Board will bear no responsibility or liability arising out of non-receipt of the same in time or otherwise.
- (3) In order to allow prospective Bidders reasonable time in which to take amendment into account in preparing their Bids, the Board at its discretion may extend the deadline for submission of the Bid.

4.0 PREPARATION AND SUBMISSION OF BID

4.1 Language

The Bid to be prepared by the Bidders, as well as all correspondence and documents relating to the Bid exchanged by the Bidder and the Board shall be written in English. Failure to comply with this may disqualify a bid.

4.2 One Bid per Bidder

Each Bidder shall submit one Bid only.

4.3 Local Representation

- a) Foreign Bidders, if they have in India a local representative in Indian / Indian agent shall indicate in their bid (Bid Proposal Sheets), the name of such person of firm and also shall furnish the following information in their bid:
 - 1) The precise relationship between the Bidder and his Indian Agent.
 - 2) The mutual interest which the Bidder and the Indian Agent have in business of each other.
 - 3) Any payment which the Indian Agent receives in India or abroad from the Bidder whether as a commission for the Contract or as a general retainer fee.
 - 4) Indian Agent's Income Tax Permanent Account Number.
 - 5) Bidder's Income Tax Permanent Account Number.
 - 6) All services to be rendered by the Indian Agent whether of general nature or in relation to the particular contract.
 - 7) All above statements have to be substantiated by authenticated documents from competent authority.
- b) Agent's commission, if any, (to be included in the Bid Price) shall be indicated separately but as a part of Bid Price and the same will be payable only in equivalent Indian Rupees. Indian agent's commission will not be subject to any escalation whatsoever and will be payable at the time of final payment after commissioning & training. To effect such payments, the Indian Agent's commission will be calculated on the basis of exchange rates (State Bank of India Exchange buying rate) as on the date of notice of the award to the successful Bidder.
- c) The bidder /Contractor shall not pay Indian Agent's Commission, unless declared in the bid.

4.4 Bid Security / Earnest Money

- (1) Pursuant to Clause 5.1 in this instruction, the Bidder shall furnish, as part of its Bid, his Bid Security EMD Rs. **65 Lakhs** in the amount **of Indian Rupees Sixty-five Lakhs only** for 15 Nos. of MCAAQMV. The Bank Guarantee (Attachment 10 of Section III, Volume-I) for Bid Security issued by a nationalized bank located in India or the private banks whose net worth is greater than Rs.4000 crores will be considered for payment of EMD through BG and same shall be submitted as per the form given with this tender document.
- (2) The Bid securities in the form of Bank Guarantee shall be valid for Two Hundred Twenty-Five (225) days from the date of opening of Techno- commercial Bids or completion of supply, installation, commissioning of all MCAAQMV whichever is earlier.
- (3) The Bid Security documents shall be uploaded through online in favour of MAHARASHTRA POLLUTION CONTROL BOARD.
- (4) Any Bid not secured by the Bid Security will be rejected by the Board as non-responsive pursuant to Sub-clause 8.4. Unsuccessful Bidder's Bid Security will be discharged or returned as promptly as possible, but not later than thirty (30) days from the expiration of the period of the Bid validity specified in Sub-clause 4.6 hereunder. The successful Bidder's Bid Security will be discharged upon the Bidder signing the Contract pursuant to Sub-clause 13.3 in this instruction and furnishing the Performance Security pursuant to Clause 14 in this instruction.
 - (5) The Bid Security may be forfeited:
 - If a Bidder withdraws it's Bid during the period of Bid validity specified in Sub-clause 4.5 hereunder;
 - b. If a bidder refuses to accept the arithmetical corrections made according to ITB (Instructions to the Bidder) Clause No. 11; also, successful bidder fails to acknowledge the receipt of LOA/PO.
 - c. In case of a successful Bidder, if the Bidder fails to sign the Contract in accordance with Sub-clause 13.3 in this Instructions and furnish Performance Security in accordance with Clause 14 in this Instructions;
 - d. In case bidder refuses to withdraw, without any cost to the Owner, those deviations, which the bidder did not state in the Deviation Schedules.
 - (6) No interest will be payable by the Board on the above Bid Security.

4.5 Validity of Bid

The bid shall remain valid and binding on the Bidder for one hundred and twenty (120) days from the final time and date for submission of the Bid. Bid validity for a shorter period shall be rejected by the Board as non-responsive.

In exceptional circumstances, the Board may in writing or by facsimile, solicit the Bidder's consent to an extension of the period of the Bid validity. If the Bidder agrees to the request for extension, the Bid Security shall also be extended for an equivalent period of time.

Any Bidder may refuse to extend the validity of his Bid without forfeiting his Bid Security, but the Bid will not be considered.

Bidders granting the requests for extension of the Bid validity will not be required or permitted to modify their Bids.

4.6 Modification and Withdrawal of Bid

- a) The Bidder may modify or withdraw its Bid after the Bid's Submission as per the conditions available at online bid submission portal.
- b) No Bid shall be allowed to be modified subsequent to the deadline for submission of Bids.
- c) No bid shall be allowed to be withdrawn in the interval between the deadline for submission of Bids and the expiration of the period of bid validity specified in the clause 4.7above. Withdrawal during this period may result in the forfeiture of the bid security pursuant to clause 4.4 (5) (a).

4.7 Rejection of Bid

Failure by the Bidder to comply with the provisions of these Instructions to Bidders or any part of the Bidding Documents may result in rejection of the Bid and forfeiture of the Bid Security.

The Board reserves the right to accept or reject any or all Bids or to amend the Bidding process at any time prior to award of the Contract without thereby incurring any liability to the affected Bidder or Bidders or any obligation to inform the affected Bidder or Bidders of the grounds for the Board's action.

The Board also reserves to itself the right of accepting the whole or any part of the Bid and the Bidder shall be bound to perform the same at the rate quoted.

4.8 Contacting the Board

Except for responses to request for clarification of the Bid by the Board, the Bidder shall not contact the Board for any matter related to this Bid from the time of submission of the Bid until the Contract is awarded.

Any efforts by the Bidder to influence the Board in his decision in respect of evaluation of the Bid or award of the Contract shall result in the rejection of the Bid and forfeiture of the Bid security.

5.0 PREPARATION OF TECHNO-COMMERCIAL BID

5.1 As per Clause number 6 (Online Bid Preparation) of Tender Notice.

5.2 Contents of Envelop "B", Qualification Documents.

Following documents shall be prepared in one (1) original and one (1) copy and be enclosed in the sealed envelope clearly marked "B" and "ORIGINAL" or "COPY" with the indication of the contents.

- 1) Authorization letter authorizing the signatory of the Bid to commit the Bidder.
- 2) Attachments in support of meeting qualifying requirements as per Clause No. 2.5 for the quoted packages (Attachments 8A, 8B & 9 of Section- III).
- Copy of certificate of local branch, sales, residential and representative office(s) of the Bidder in India as per certificate from pursuant to Attachment 2 of Section III.
- 4) CertificateofletterofauthorityfrommanufacturersforalltheEquipment (Attachment 3 of Section III).
- 5) Certificate from manufacturer stating the country of origin of each Equipment duly authenticated by competent authority of that country (Attachment 4 of Section III).
- 6) Certificate of carrying out O&M by O&M Partner (Attachment 5 of Section III).
- 7) List of Equipment offered (Attachment 6 of Section III).
- 8) List of Manufacturers of the equipment offered (Attachment 7 of Section III).
- 9) Pre-requisite for installation of equipment offered (Attachment 11 of Section III).

5.3 Contents of Envelop "C"; Techno-commercial bid including Technical Specifications and catalogues

The following documents shall be enclosed in the sealed envelope marked "C" and "ORIGINAL" or "COPY" with the indication of the contents. The Bidder shall prepare one (1) original and one (1) copy.

1) Attachments 1 & 2 of Financial Bid, Section IV must be submitted through online.

- 2) Deviation Schedule (Attachment 12 of Technical Bid, Section-III).
- 3) Technical Data sheets of the Equipment in the package (Annexure-I, Vol. II) offered:
 - a) In case that there is no deviation from the Board's requirement, the Bidder must write down "complied" in the column for "Bidder's Response" and it is not necessary to rewrite the same words of the requirements unless there is over specification points are available with the items offered. If, not found document evidence to support writing "complied" such bid shall be rejected and bidders EMD will be forfeited.
 - b) In case of any deviation from the requirement the Bidder must write down the "not complied" & the deviation in blanks under "Bidder's Response".
 - c) The Bidder shall clearly indicate contents and quantities of standard accessories for the proposed Equipment in the blanks.
 - d) The Bidder shall understand that decision of the Board will be binding in regards of anything not specifically mentioned in the technical specification.
 - e) The Bidders shall offer only one manufacturer, one brand and one model per parameter.
 - f) Complete set of original catalogues and /or photographs and/or pamphlets illustrating principal feature.

6.0 PREPARATION OF FINANCIAL BID

6.1 As per Clause number 6 (Online Bid Preparation) of Tender Notice.

6.2 Bid Form

There would be two different financial Bids: One for a Vehicle (TATA LPT 709Ex 2 or its equivalent, BS-VI variant) with necessary chassis build up with a thermally stable cabin, where all the continuous air quality monitoring analysers and its necessary supporting system AND another for Continuous Ambient Air Quality Monitoring Analysers System. The final financial bid price would be considered as the total of these two bids.

The Bid Prices to be quoted by the Bidder shall be prepared on the official letter head of the respective Bidder according to the Attachment 1 "Bid Form" in Section IV without any alteration or change. (Attach Scan Copy Online in Financial Bid)

The Bid Prices shall be quoted for performing the Contract strictly in accordance with the Technical Specifications.

The Bid Prices quoted by the Bidder shall be firm during the Bidder's performance of the Contract and not subject to variation on any account.

A Bid Price submitted online with an adjustable price will be treated as non-responsive and will be rejected.

6.3 Summary of Bid Price

Summary of Bid Price shall be prepared and submitted online in accordance with the Attachment 2 in Section IV.

The Bidder shall indicate prices online for the package in the following manner:

- (i) For the Goods Supplied from Foreign Origin
 - 1. CIF Price at Port of de-embarkment.
 - a) FOB Price of the Package (for the equipment to be supplied from Foreign Origin)
 - b) Freight for complete Package
 - c) Insurance covering all risks up to Port of de-embarkment
 - 2. Local Costs
 - a) Cost of
 - a) Port handling and clearance charges.
 - b) Transportation cost from the port to Port of deembarkment to Sites.
 - c) Insurance covering all risks from Port of de-embarkment up to handing over.
 - d) Installation and commissioning.
- (ii) For the Goods Supplied from India
 - a) The price of the Equipment quoted ex-works, ex-factory, exwarehouse, ex-showroom, or off-the-shelf including all customs

duties and sales and other taxes already paid or payable on the components and raw material used in the manufacture or assembly of the Equipment quoted ex-works or ex-factory.

- b) Price for handing and inland transportation, insurance up to handing over the equipment at Site and other local costs up to delivery of the Equipment to each Site.
- c) Cost of TATA LPT 709Ex 2 or its equivalent, BS-VI variant along with vehicle frame (Chassis build up) air conditioned and thermally stable instrument cabin.
- c) Installation and commissioning
- d) Price of other incidental cost, if any. Then the Bidder shall specify the same.
- (iii) Price of other incidental cost such as Indian Agent's Commission, if any. The Bidder shall specify the same.
- (iv) Cost of O&M of Continuous Ambient Air Quality Monitoring Analyser System for Five (5) years including insurance.

(v) Training

The Bidder shall provide training as indicated in clause 10 of S/W.

Cost of Travel, Boarding & Lodging and local transport cost of participants shall be borne by the supplier.

Note:

- Quoted cost O&M of a Continuous Ambient Air Quality Monitoring Analyser System and mobile vans for each year should be at least 12% of the cost of Supply & installation of the Continuous Ambient Air Quality Monitoring Analyser System. In case the bidder quotes O&M cost lower than 12 % of the Supply & installation cost, the Owner will reduce the Supply & installation cost suitably, so as to make the O&M cost as 12% of the Supply & installation cost, keeping the total quoted cost as unchanged.
- (2) All the local taxes & duties applicable in the State of India i.e. Custom Duty, GST and other taxes etc. which will be payable on the Equipment if the Contract is awarded shall be paid extra as actual by the Board.
 - (3) All taxes as applicable shall be paid extra as actual by the Board.

6.4 Bid Price Breakup

The Bidder shall prepare and submit online the Bid Price Breakdown (CIF Price or Ex-works price as applicable) for each item of the quoted package(s) in accordance with Attachment 3 in Section IV.

The Bidder shall prepare and submit online break up of Operation & Maintenance of Continuous Ambient Air Quality Monitoring Analyser System as per Attachment 3A in Section-IV.

6.5 Currencies of Bid:

The unit rates and the prices shall be quoted by the bidder separately in any one of International trading currencies for the equipment, which the bidder proposes to Supply. {Euro (EUR), Great Britain Pound (GBP), Indian Rupee (INR), US Dollar (USD), Japanese Yen (YEN)}

7.0 COMPLETION AND SUBMISSION OF BID ONLINE

7.1 Completion of Bids

7.1.1 Techno-commercial Bid

(1) The Techno-commercial Bid shall not contain any information regarding Bid Prices and other financial matters except the Bid Security pursuant Clause 4.4 in this instruction.

7.1.2 Financial Bid

The financial bid must be submitted online as per price bid(s) Prescribed at Sub-clauses 6.2, 6.3, 6.4 and 6.5.

7.1.37.1.3

- (1) In case of discrepancy between "ORIGINAL" and "COPY" bids prepared pursuant to clause 5 in this instruction, the ORIGINAL" shall govern.
- (2) The original and the copy of the Bid shall be typed or printed in indelible ink and shall be signed by the Bidder or a person or persons duly authorized to bind the Bidder to the Contract. All pages of the Bid except for un-amended, printed literature, shall be initiated by the person(s) signing the Bid.
- (3) Any interlineations, erasures or over writing shall be valid only if they are counter signed by the person or persons signing the bid with official stamp. A list of such occurrences is to be brought out in separate sheet including Section number. Clause number and Page number and submitted along with the respective envelope of Techno-commercial and/or financial bid.

(4) The Bid shall be signed by the Bidder himself or for and on behalf of the Bidder by an officer or officers with authorization letter as the case may be. A notarized copy of such Power of Attorney shall be submitted with the Bid pursuant to Clause 5 in this instruction.

7.2 Submission of Bid

Bids shall be submitted online only.

All the documents for the Techno-commercial Bid shall be submitted as per Clause number 6.0. Also, hard copies of supporting documents of Technical Bids shall be submitted manually to MPCB on opening of Technical Bids and the bids shall be addressed to:

The Member Secretary,
MAHARASHTRA POLLUTION CONTROL BOARD,
Kalpataru Point, 3rd Floor, opp.
Cine planet, Near Sion Circle, Sion, (East), Mumbai – 400 022.

The Bids received after the specified time and date here above for whatever reason shall be not accepted online by the system.

.

Bids in the form of Telex, facsimile, telegraph or email, will not be accepted. Only the complete **Techno-commercial Bid** documents specified above, shall be submitted through online.

The Bids once opened shall not be returned to the Bidders regardless of the result of the Bid. This will apply to both the Techno-commercial and financial bids in case a bidder is not qualified at the stage of Techno commercial evaluation.

8.0 OPENING AND EVALUATION OF TECHNO-COMMERCIAL BID'

8.1 Opening of Technical Bid

Only the Technical Bid will be opened in public at MPCB, Head Office as per Tender schedule. Bidders or their representatives may attend the opening. During opening of the Techno-commercial Bid, the Bidder's name, the presence or absence of necessary envelopes, withdrawals of the Bid and such other details as the Board at their discretion may consider appropriate will be announced and recorded.

All the Bidders or their representatives present shall sign a format evidencing their attendance.

8.2 Confidentiality of the Process

Information relating to the examination, clarification, evaluation and comparison of Bids and recommendations for the award of the contract shall not be disclosed to bidders or any other person not officially concerned with such process. Any effort by a bidder to influence the Board's processing of Bids are award decisions may result in the rejection of the Bidder's Bid. The request for clarification and response shall be writing or by fax, but no change in the price or substance of the bid shall be sought, offered or permitted except as required to confirm the correction of arithmetic errors discovered by the Board in the evaluation of the bids in accordance with the clause

11.2 of these instructions.

8.3 Clarification of Techno-commercial Bids

To assist the Techno-commercial examination and evaluation of bids, the Board may, at its discretion ask the bidder for a clarification of its Techno-commercial bid. **A pre bid meeting may be called.** All responses to request for clarification shall be in writing, and **no change in the price bid shall be sought, offered or permitted.**

8.4 Preliminary Examination

The Board will examine the Techno-commercial Bids to determine whether they are complete, whether the documents have been properly signed and whether the Techno-commercial Bids are generally in order. Any Techno-commercial Bid found to be non-responsive for any reason i.e. non-conformity of bid security, or not meeting the eligibility criteria and/ or qualifying requirements pursuance to clause 2.4 & 2.5 of ITB etc. will be rejected by the Board. No further Techno-commercial evaluation shall be carried out for such bidders.

Prior to detailed evaluation of Techno-commercial bids, pursuant to clause 8.5, the Board will determine the substantial responsiveness of each Bid to the Bidding Documents including acceptable quality of goods offered pursuant to clause 2.4 & 2.5. A substantially responsive Bid is one, which conforms to all terms and conditions of the Bidding Documents without material deviations, objections, conditionality or reservations. deviation, objection, conditionality or reservation is one (i) that affects in any substantial way the scope, quality or performance of the contract; (ii) that limits in any substantial way, inconsistent with bidding documents, the Owner's right or the successful Bidder's obligations under the Contract; or (iii) whose rectification would unfairly affect the competitive position of other Bidder's who are presenting substantially responsive bids.

No deviation, whatsoever, is permitted by the Owner to the provisions relating to the following clauses (important Conditions):

- (a) Bid security (ITB Clause 4.5)
- (b) Resolution of Disputes (G.C.C clause 37),
- (C) Applicable law (G.C.C clause 42),
- (d) Taxes & duties (G.C.C Clause 38),
- (e) Performance security (ITB Clause 14 & GCC Cl.28),
- (f) Force Majeure (G.C.C Clause 35).

A bid with deviation to any of the above clauses (important Conditions) will be liable to be rejected.

The Owner's determination of bid's responsiveness is to be based on the contents of the bid itself without recourse to extrinsic evidence. If a bid is not substantially responsive, it will be rejected by the Owner, and may not subsequently be made responsive by the Bidder by correction of the non-conformity.

8.5 Evaluation of Techno-commercial Bid

- (1) The Board will determine the responsive Techno-commercial Bids for the opening of Financial Bid if the Techno-commercial Bid meets satisfactorily technical specification and any other information, which they consider relevant to his offer.
- (2) If a Bidder is found not substantially responsive to the technical requirement, the Techno-commercial Bid will be rejected and the subsequent information as to opening of the Financial Bid will not be notified.
- (3) If the Techno-commercial clarifications are required by the Board to any part of the Techno-commercial Bids, the Bidders will be requested to clarify the same in writing.
- (4) If only ONE Bidder is qualified in the Technical Bid, the Board will have the right to go ahead for the Financial Bid opening of Single Technically Qualified Bid and accept it if, the price band offered by the bidder is acceptable to the Board.

8.6 Evaluation Criteria of Techno-commercial Bid

The Bidder who fulfil the requirements specified under Qualification Requirement (**Clause 2.5**) will be short listed. Under the Qualification Requirement a minimum threshold limit has been set for each parameter like technical experience and financial strength. Bidders not meeting the minimum threshold limit in any of these parameters will not be short-listed.

The detailed techno-commercial evaluation to be carried out shall be restricted to these short-listed Bidders only.

9.0 NOTIFICATION OF SUCCESSFUL TECHNO-COMMERCIAL BID

After completing the techno-commercial evaluation of the Techno-commercial Bid first, accordingly **pre-qualified and techno-commercially responsive Bidders** will receive online communication **before** opening of the Financial Bid.

10. OPENING OF FINANCIAL BID

The Bidders to whom the opening time, date and venue for the Financial Bid are notified by the Board in writing will be invited to attend the Financial Bid opening. The Bidder's representatives present shall sign a format evidencing their attendance.

During opening of the Financial Bid, the Bidder's name, quoted price of package and other details as the Board, as its discretion may consider appropriate will be announced and recorded.

11. EXAMINATION OF FINANCIAL BID

11.1 After opening of the Financial Bid, the Board will examine them to determine whether they are complete, signed, generally in order and substantially responsive to the Bidding Documents or not.

A Financial Bid determined as being not substantially responsive will be rejected.

The Board may waive any minor informality or non-conformity or irregularity in a Financial Bid which does not constitute a major deviation or reservation provided such waiver does not prejudice or affect the relative ranking of any Bidder.

If there is any discrepancy between words and figures, the amount in words will prevail. The Financial Bid which is incomplete or conditional will be rejected.

- 11.2 During examination of Financial Bid any **arithmetical errors** will be corrected as follows:
 - a) If there is a discrepancy between the unit price and the total price per item that is obtained by multiplying the unit price and quantity, the unit price shall prevail and total price per item will be corrected. If there is a discrepancy between the Total Amount and the sum of the total price per item, the sum of the total price per item shall prevail and the Total Amount will be corrected accordingly.
 - b) The amount stated in the Form of Bid shall be adjusted by the Board in accordance with the above procedure for the correction of errors and, shall be considered as binding upon the bidder. If the bidder does not accept the corrected amount of bid, its bid will be rejected, and the bid security will beforfeited in accordance with clause 4.5 (5)

12. EVALUATION AND COMPARISON OF FINANCIAL BID

12.1 Evaluation Procedure

The Board will evaluate the Bid previously determined to be Techno – commercially responsive pursuant to clause 8.6. The Board reserves the right to reject any bid or bids received at its discretion without assigning any reason whatsoever.

- 12.2 The purchaser's evaluation of a bid will take into account following factors:
 - I. Total cost of Supply, installation & Commissioning at the identified city / location of the equipment as below:
 - 1) The CIF port of entry price of the equipment to be offered from abroad.
 - 2) The ex-factory/ ex-warehouse/ off the shelf price of the equipment to be offered from within India (such price include all costs as well as duties and taxes paid or payable on components and raw material incorporated or to be incorporated in the equipment)
 - 3) Local costs i.e.
 - a. Cost of TATA LPT 709Ex 2 or its equivalent, BS-VI variant along with vehicle frame (Chassis build up) air conditioned and thermally stable instrument cabin.
 - b. Cost of port handling and custom clearance,
 - c. Transportation cost from Port of de-embarkment to Sites,
 - d. Insurance from Port of de-embarkment up to handing over and
 - e. Installation and commissioning charges at site.
 - 4) Other incidental costs, if any (such as Indian agent's commission)
- II. O & M cost (including insurance) for five years as Net Present Value Discounted @12% per annum.

NOTE: Taxes and duties shall not be considered for the purpose of evaluation.

12.3 The Board will evaluate and compare Bid for complete package.

12.4 The rate of exchange for evaluation

To facilitate evaluation and comparison, the Owner will convert all Tender prices to Indian Rupees at the BC selling exchange rate as determined by the State Bank of India, on the date of opening of Techno-commercial Bids.

12.5 Clarification on Financial Bid

For the purpose of examination, evaluation and comparison of the Financial Bid, the Board may at his discretion request the Bidder in writing to clarify his Financial Bid, but no change in the Bid Price or substance of the Bid will be sought, offered or permitted.

12.6 Cost Compensation for deviations

Deviations specifically declared by the bidders in respective Deviation Schedule (Attachment 12 of Technical Bid, Section – III) only will be taken into account for the purpose of evaluation.

In case of any of these deviations are not acceptable to the Owner, the Bid shall be rejected.

In case any of the deviations are acceptable to the Owner, the Owner will make its own assessment of the cost of these deviations and consider it for evaluation for the purpose of ensuring fair comparison of bids.

Bidders may note that all deviations / variations and additional conditions etc. found elsewhere in the bid other than those stated in the Deviation Schedules, save those pertaining to any rebates, shall not be given effect to in evaluation and it will be assumed that the bidder complies to all the conditions of Bidding Documents. In case bidder refuses to withdraw, without any cost of the Owner, those deviations, which the bidder did not state in the Deviation Schedules, the bid shall be rejected and the bid security of the bidder may be forfeited.

13. AWARD OF CONTRACT

13.1 Award of Contract to Successful Bidder

The Board will award the Contract to successful Bidder:

- 1. Whose Bid will be determined to be substantially responsive to this Bidding document and who will be determined by the Board, to be qualified technically, financially and otherwise in respect of such other capabilities, as the Board may be deem necessary and appropriate to satisfactory performance of the Contract and
- Whose Bid will be determined to be lowest evaluated, responsive
 Bid and is determined to be qualified to satisfactorily perform the contract.
- 3. The Board reserves the right to reject any bid or bids received at its discretion without assigning any reason whatsoever.

13.2 Notification to Award

Prior to the expiration of the Bid validity pursuant to sub-clause 4.6 in this Instructions, the Board will notify the successful Bidder in writing by registered letter or by facsimile to confirm that it's Bid has been accepted. The notification of award will constitute the formation of the Contract.

Upon the successful Bidder's furnishing of the Performance Security pursuant to Clause 14 the Board will promptly notify each unsuccessful Bidder and will discharge their Bid Security pursuant to Sub-Clause 4.5.

13.3 Signing of Contract

Within Thirty (30) days of the receipt of notification of award from the Board, the successful Bidder shall sign and date of Contract. The Contract shall take the form of General and Special Condition attached to Section V, VI and such modifications as may be necessary. The Bidder shall prepare at his own cost one (1) original and three (3) bound copies of the Contract including the Contract Form attached to the Special Conditions of Contract (Attachment 3 of Section VI) for distribution to the parties concerned.

14. PERFORMANCE SECURITY

Within thirty (30) days of notification of award from the Board, the successful Bidder shall furnish the Performance Security in the form of bank guarantee issued by a reputable bank (as per enclosed list of Attachment – 15) having license to do business in India in accordance with Attachment 1 of Section VI "Performance Security Form" provided in Special Conditions Contract for an amount equivalent to 10% (ten percent)of the Contract Price, for one year after successful commissioning of system.

Failure of the successful Bidder to comply with the requirement of Sub-clause 13.3 or Clause 14 in these instructions shall constitute sufficient grounds for the annulment of the award and forfeiture of the Bid Security in which event the Board may make the award to the second-high ranked Bidder or call for new Bids.


15. EXPENSE OF BID

Under no circumstances will the Board be liable to the Bidder for any expenses, losses or damages whatever incurred in the Bid including but not limited to expenses, losses or damages associated with preparation of the Bid, visits to the Sites and all matters in connection with the Contract negotiation sand signing regardless of the conductor outcome of the bidding process.

16. RESPONSIBILITY FOR INFORMATION SUPPLIED

Prior to the final time and date for submission of the Bids, no representation, communication, explanation or statement, verbal or written, made to the Bidder or anyone else by the Bidder or any of their employees or authorized representatives other than as may be set out in amendment issued in accordance

	h Sub-clause 3.6 in this Instructions shall bind the wers and duties under the Contract.	e Bidder in the exercise of their
	information given in the Bidding Documents is the different of the Board does not hold himself responsi	
Supply, insta	stallation and commissioning and Operation & maintenance services of Mobile Continuous	s Ambient Air Quality Monitoring Van (MCAAQMV)

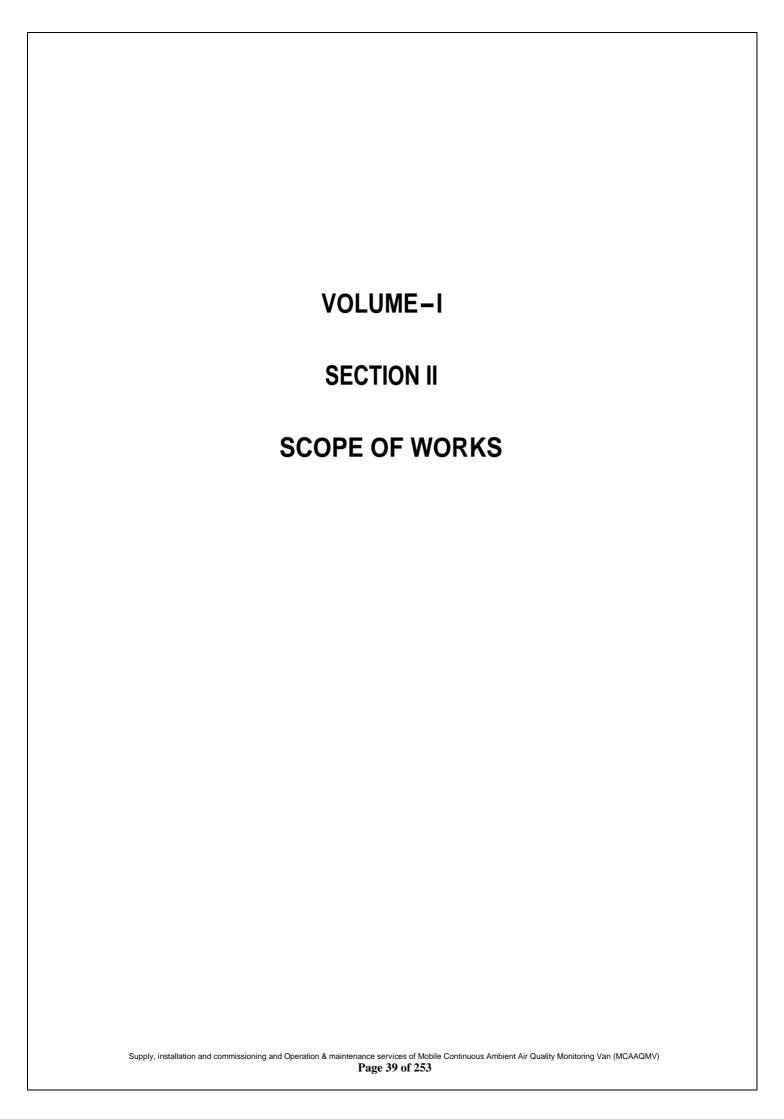

Sr No Details Page No. 1. 2. Scope of Services......43 3. Minimum Specifications......43 4. Desired Output for AAQMS Equipment......43 5. Location46 6. SUPPLY of Equipment......46 7. 8. Installation of Equipment......46 9. 10. Provision of Training48 11. Operation & Maintenance of Air Monitoring Systems51-52 Attachment 1 Equipment List......55 Attachment 2 Protocol Manual Calibration56 to 57 Daily Reporting Format for Meteorological Parameters ... 58 Attachment 3 Monthly Reporting Format for Meteorological Parameters 59 Attachment 4 Pollutants......60 Attachment 5 Daily Reporting Format for Main Attachment Monthly Reporting Format for Main Pollutants61 6

1.0 <u>DETAILS OF PROJECT STRUCTURE</u>

- (a) The Monitoring Van designed to be used for monitoring of ambient air quality. This shall build on Tata Cabin Chassis model TATA LPT 709Ex 2 or its equivalent, BS-VI variant with driver cabin and Instrument Cabin. The Instrument Cabin shall be air conditioned and able to maintain constant temperature, so that the analysers are easily accessible front and back for calibration and maintenance.
- (b) Successful Bidder would be awarded the project/work under a Supply and Service Agreement, which would entail:
- Supply of Vehicle model number TATA LPT 709Ex 2 or its equivalent, BS-VI variant (15nos.): The procurement of 15 numbers of Vans along with chassis (Vehicle Frame) and Supply, installation and Commissioning of One Set of air quality monitoring analysers system will be in the scope of the bidder. The Bidder would provide complete set of Mobile Continuous Ambient Air Quality Monitoring Van ready to monitor the continuous ambient air quality wherever required.
- 2. Supply, installation and Commissioning of One Set of MCAAQMV at the defined cities/ locations.
- 3. Operation and Maintenance of the Analysers Systems for a period of 5 years from the date of its commissioning
- 4. MPCB would make payment for MCAAQMV as per schedule of requirement, for Supply, Installation and Commissioning of the system. MPCB would procure all the MCAAQMV equipment on its name. MPCB will make regular payments for the O&M at the end of each Quarter. The bidders therefore need to quote three prices for;
 - (a) Supply of TATA LPT 709Ex 2 or its equivalent, BS-VI variant (total 15 nos.) along with chassis (Vehicle Frame) to be used as instrument cabin (air conditioned) and ready for analysers to be fitted in the instrument cabin.
 - (b) Supply, Installation and Commissioning of the analysers system, total of 15 Nos. each in each MCAAQMV as per invitation for bids section.
 - (c) Reporting of data to MPCB. The price for the data Supply would include the Operation and Maintenance, including incidental charges, providing manpower at site, etc.

These vans will be stationed at Regional Offices of MPCB. Bidder would bear the initial installation and commissioning cost for these facilities and the monthly recurring cost pertaining to their usage (monthly telephone) would also be borne by the Successful Bidder.

(b) SCHEDULE OF REQUIREMENTS

The MCAAQMV shall have the following schedule of requirement. The system should be completely functional. Any balance of material not specified but required for the purpose must be supplied by the bidder.

Schedule No.	Brief Description	Qty. in nos.
1.	Continuous Automatic Air Quality Monitoring Analysers for CO, SO ₂ , NO-NO ₂ -Nox, O ₃ and Beta Gauge PM _{2.5} and PM ₁₀ Monitors	1 unit each
2.	BTX Analyser	1 Unit
3.	Multi-calibration systems for gaseous monitors SUPPLY /generation and automated calibration	1 Unit
4.	Sensor based single instrument to measure Meteorological parameters comprising Wind Direction, Wind Speed, Ambient Temperature, Relative Humidity, Solar Radiation and Rainfall mounted on telescoping crank up meteorological Mast	1 Set
5.	Computer system consisting of one PC along with Laser Printer and DAS at the monitoring station and One PC at central office with peripherals for transferring of data and system integration, telephone	1 Lot
6.	Modem / Dongle for internet connectivity	2 Units
7.	Arrangements like Thermally Stable Housing (Body Built up) for installation of Continuous Ambient air quality Monitoring analysers with Sampling line, Internal fitting, Instruments racks, Electrical and Gas line Fittings, Tools (electrical and mechanical).	1 Unit
8.	Split Air Conditioners (2 Ton capacity)	2 Units
9.	Petrol Generator set- 6.5 KVA	1 Unit
10.	5 KVA Stabilizer	1 Unit
11.	Vehicle model number TATA LPT 709Ex 2 or its equivalent, BS-VI variant along with vehicle frame (Chassis build up) air conditioned and thermally stable instrument cabin.	1 Unit

2.0 SCOPE OF SERVICES

The Scope of Works under the package shall include:

- A) Vehicle model number TATA LPT 709Ex 2 or its equivalent, BS-VI variant along with vehicle frame (Chassis build up): The Monitoring Van designed to be used for monitoring of ambient air quality. This shall build on Tata Cabin Chassis model TATA LPT 709Ex 2 or its equivalent, BS-VI variant with driver cabin and Instrument Cabin. The Instrument Cabin shall be air conditioned and able to maintain constant temperature, so that the analysers are easily accessible front and back for calibration and maintenance
- B) Supply of CAAQMS Analysers: The Supply including packing, transportation, insurance, custom clearance, port clearance and handling, inland transportation, inland transit insurance and delivery to site, installation, testing and commissioning of equipment and provision of training of MPCB officials' station wise.
- C) O & M of CAAQMS Analysers and Mobile Vehicle: Operation & Maintenance of Air Monitoring Systems along with Mobile Vehicle for a period of five (5) years from the date of commissioning of the station, which can be extended up to three (3) years at the mutually agreed rates and terms and conditions.
- D) Data & Report of data pertaining to MCAAQMV to MPCB.
- E) Online transfer of data to MPCB and CPCB and establishing connectivity to AQI server at MPCB and CPCB.

Other services involved with performance of the Works are specified in General and Special Conditions of Contract of bid document.

3.0 MINIMUM TECHNICAL SPECIFICATIONS

The minimum technical specification requirements for the MCAAQMV to be commissioned and installed are given in Volume - II (Technical Specifications) of bid document. However, the actual technical proposal can have higher or better technical performance parameters and the minimum specifications proposed should not be taken as a constraint on the upper side. The technical specifications given in Volume - II (Technical Specifications) of bid documents are descriptive and Selection Committee can consider technical proposals having similar specifications. There will not be any changes in the technical specification.

4.0 DESIRED OUTPUT FOR MCAAQMV EQUIPMENT

The desired output requirements from the MCAAQMV equipment to be installed at are given in Attachment 2 to 6 of Scope of work of bid document.

5.0 DATA MANAGEMENT AND QUALITY CHECKS

Data shall be collected and validated according to USEPA standards/ National Ambient Air Quality Standards using the methodologies included in 40 Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design.

Successful bidder shall submit a Standard Operating Procedure for the air quality monitoring van to the Board before award of contract. This Standard Operating Procedure shall be approved by the Board prior to award. The Standard Operating Procedure shall contain the following:

- Operating procedures for all analyzers and meteorological sensors
- Calibration procedures
- Calibration schedule
- Maintenance procedures
- Maintenance schedule
- Data validation procedures
- Data reporting as per attachment X1 to X5
- Data obtained from these calibration checks and copies of associated Quality Assurance and calibration documentation, shall be submitted to the Board along with the Air Quality Data.

Upon 3 days' notice from the Board once per year, Successful Bidder shall agree to submit to an audit of calibrations, conducted, using preapproved US EPA methodologies, by a third party. Third party audit may be arranged by the Owner (MPCB) by the agency decided by them, at their cost and bidder shall provide all necessary facilities to carryout required audit. The results of these audits shall be made immediately available to both the Seller and Buyer.

GENERAL GUIDELINES

Working Hours: The site for MCAAQMV operation should be manned by the employees (Engineer) of the Successful Bidder. The van will be in operation as and when needed by respective Regional Officers.

Insurance: Successful Bidder would initially bear the cost of insuring the vehicle, equipment (Comprehensive) and facilities against any theft, fire and other applicable provisions during tenure of contract period including O & M with a copy to MPCB of an appropriate amount. Board shall reimburse the same to the successful bidder on submission documentary proof. However, insurance during commissioning shall be borne by the bidder.

Station telephone / modem arrangement:

The successful bidder shall arrange telephone connection modems etc. required for the smooth Operation of the station. The necessary documentation shall be provided by the concerned MPCB / local authority of the board.

6.0 LOCATION

The MCAAQMV will be located at each of the Regional Offices of MPCBoard. As per the Invitation for Bids (Tender notice - Page no. 16)

7.0 SUPPLY OF EQUIPMENT

Attachment-1, specifies the list of equipment in the package, quantity of equipment to be supplied, delivered and installed.

8.0 INSTALLATION OF EQUIPMENT

All the necessary arrangements and adjustments for suitable commissioning, installation and operation of the equipment shall be made by the Bidder including commissioning of vehicle frame (Chassis build up), telephone/mobile/internet connection, however all the required document shall be arranged by the Board.

9.0 INSPECTION AND TEST

9.1 Unpacking Inspection

The Contractor shall inspect at Site whether all the Equipment are packed in conformity with the Equipment list and packing list without any damage immediately after arrival of the Equipment at each Location.

9.2 Performance Test

The Contractor shall carry out the performance test for all the Equipment supplied under the scope of work of this document in presence of agency / expert / committee members appointed by the Member Secretary, MAHARASHTRA POLLUTION CONTROL BOARD.

In case the Equipment for performance test requires the supplemental and/or supporting Equipment, the Contractor shall carry out the performance test including such Equipment.

10.0 PROVISION OF TRAINING

The supplier shall provide the training to the Board staff for minimum two (2) weeks to three (3) persons per site (maximum) after the performance

test and commissioning. Training should include but not limit to the following:

- 1) Inspection of the Equipment.
- 2) Precautions in use of the Equipment.
- 3) Basic measurement principle.
- 4) Principles of operation of the Equipment.
- 5) Start-up and shutdown procedure.
- 6) Operation of the Equipment.
- 7) Calibration method.
- 8) QA/QC.
- 9) Data Validation & management and software application.
- 10) Safety precautions.
- 11) Basic maintenance procedure.
- 12) "Do's" and "Don'ts" in operation of the Equipment.
- 13) Handling of hazardous chemicals and gas.
- 14) Others, which are deemed to be necessary by the Supplier.

In case the Equipment for training requires the supplemental and/or supporting Equipment, the Supplier shall carry out the training including such Equipment.

The Supplier shall discuss and finalize the detailed contents and schedule of the training program in consultation with the Board during installation of the Equipment.

The Supplier shall furnish the training manual and/or CD as required for training for all the Equipment supplied under the scope of work of this document.

Contents of training manual and/or CD for the Equipment are as follows:

- 1. Principle of the Equipment.
- 1. Operation and calibration of the Equipment.
- 2. Maintenance and basic repair of the Equipment.
- 3. Safety instruction of the Equipment.
- 4. Others, which are deemed to be necessary by the Supplier.
- 5. QA/QC, Data Validation &management and software Application

11.0 Operation & Maintenance of MCAAQMV

- 11.1 The Contractor's responsibilities shall include without limitations the following works to be carried out on the MCAAQMV installed under this Contract during the Operation & Maintenance of the complete System:
 - a) Operation and Maintenance of all the commissioned equipment and amenities as supplied by the Manufacturer under the Contract including

services during forced and planned outages and overhauls.

- b) The Operation and Maintenance of the vehicle would be carried out by the supplier. This maintenance will be as per the specifications / schedule specified by the manufacturer/as specified by the Board.
- c) The Contractor shall take over the entire MCAAQMV (including all equipment) for O&M after execution of Indemnity Bond as per format placed at <u>Attachment- 13</u>, <u>Section III</u> of bid document.
- c) The Contractor shall provide to the owner a monthly summary of all operation and maintenance activities performed by the contractor during each month.
- d) Operation and Maintenance Obligations:

In implementing its obligations to operate and maintain the facility under this Contract, the Contractor shall:

- i) Under take comprehensive maintenance including i.e. schedule and breakdown maintenance & repair at site and keep Board Informed regarding status of vehicle & equipment and forward daily data as per Attachment 3 & 5 of Section - II.
- ii) The Operation and maintenance of the Mobile vehicle along with chassis build-up (TATA LPT 709Ex 2 or its equivalent, BS-VI variant along with vehicle frame (Chassis build up) air conditioned and thermally stable instrument cabin) would be the responsibility of the supplier and would ensure the maintenance of the vehicle as per the standard procedure / schedule prescribed by the manufacturing company and as per the laid out standards in the operating manual of the vehicle.
- iii) Obtain permission from the owner and inform the O&M for any assistance for which equipment is required to be sent to the works.
- iv) Take reasonable action to assure that the Personnel deployed at Air Monitoring Vans and any subcontractors and agents are provided with a work place in compliance with applicable Law.
- v) Keep the Air Monitoring Van clean, well maintained inside and in good working condition.
- vi) Security: It is the duty of the Contractor to secure the movable, immovable and other properties of the Owner at the Air Monitoring Station. The Contractor shall indemnify the loss caused to the Owner on account of any damage, loss or theft caused to the property of the Owner.

- vii) Scheduled Maintenance: Unless Owner and Contractor mutually agree otherwise, perform all required Scheduled maintenance for all equipment, auxiliaries etc., in accordance with the O&M specifications.
- viii) Unscheduled Maintenance: Perform all Unscheduled Maintenance and repairs for all equipment, auxiliaries etc. within (24) hours of the occurrence of the event requiring Unscheduled Maintenance, the operator shall provide the Owner with detailed written information on nature of the repair or replacement to be carried out, estimated down time and other necessary details as required.
- ix) The Contractor shall source all the spares required for maintenance & repairs of the installed equipment from O&M only.
- e) The Operator shall not:
 - i) Make any modifications as to the Air Monitoring Van, other than in an Emergency, without the prior written approval of the Owner, or
 - ii) Dispose of any assets, settle law-suits or engage in transactions relating thereto on the Owner's behalf without the prior written approval of the Owner.
- f) The Contractor shall purchase spare parts, materials, supplies and other consumable items, and maintain an inventory thereof, for the Air Monitoring Systems. All such material supplied and other items shall be the property of the Contractor However all the spares shall be sourced from OEM's only.
- g) The Contractor shall review all applicable Laws and initiate and maintain such prosecution, procedures and operating plans relating to operation of the Air Monitoring Systems as are necessary to comply therewith or assist the owner in complying therewith as the case may be.
- h) The Contractor shall operate the equipment as per the laid out standards in the operating manual of the equipment and providing data for ambient air to MPCB on daily basis in the suggested format. The daily monthly and yearly Reporting Formats are attached **Annexure X1 to X5**
- i) Provide data collected through operation of the equipment on daily basis in suggested output formats given in the bid document.
 - i) Establish and maintain a daily and monthly and yearly reporting system to provide storage and ready retrieval of operation and maintenance data including such information necessary to verify calculations. The

monthly reporting shall contain variances from targets.

- ii) Provide access to the owner to the Air Monitoring Vans and its data at all reasonable times and as and when required.
- iii) Provide the operational date required to all competent authorities including, Government of India or concerned State Governments.
- iv) Online transfer of data to MPCB/CPCB server and AQI server.
- k) The Contractor shall ensure accuracy of the data provided as per standards.
- The contractor shall ensure periodic re-calibration of all the equipment as per manufacturer's instructions and maintain "Protocol Calibration" as per Attachment 2 of Section II.
- **11.2** Owner shall arrange for the following and Contractor shall guide and assist the Owner:
 - a) The Owner shall pay O&M charges to the Contractor at the end of each quarter after submission of validated data & report by the Contractor, in accordance with the payment terms detailed in Special Conditions of Contract.
 - Owner shall pay all fees including Service Tax, etc., imposed upon Owner by the Applicable Law.
 - c) Spare parts/ consumable replacement document is maintained and verified by the owner/ board. The contractor has to maintain records / Receipts/ bills paid available as and when required
- 11.3 Handing Over of Mobile Van: On expiry/closure/termination of the Contract Agreement, Vans shall be handed over to Board in working condition to the satisfaction of Board. Few or all the spares procured by the Contractor and unused as on date of handing over may be purchased by the Owner at his discretion provided Contractor is able to provide reasonability of the costs of such spares. In addition, the Contractor shall provide consumables equivalent to three months consumption on expiry/closure/termination of the Contract Agreement without any extra financial implication.

11.4 Penalties:

During O&M period, in case of any Analyses/ system failure, penalty will be charged by MPCB @ Rs.1,000/- (one thousand) per day per Analyzer after a grace period of seven (7) continuous non-working days. The grace period of seven (7) continuous non-working days shall be given only once per quarter (3 months).

Total penalty per year during O&M period on account of above conditions shall be limited to 30% of total O&M charges for one year. Failing which defective/ malfunctioning Analyser / system has to be replaced.

In case penalty in the year exceeds 30% as above, the Contractor shall be required to replace the defective analyser (s) or systems with new ones at his own cost, failing which the MPCB shall have the right to terminate the O&M contract and forfeiture of BG.

12.0 SCHEDULE

- 12.1 Contractor shall complete all activities covered in the scope of work up to installation & commissioning of Mobile Continuous Ambient Air Quality Monitoring Vans within 180 days from date of opening of Letter of Credit.
- The Contractor shall carryout Operation & Maintenance of Air Monitoring Systems along with Mobile Vehicle for a period of five (5) years from the date of commissioning of the system, which can be extended up to three (3) years at the mutually agreed rates and terms and conditions.
- 12.3 The operation and maintenance contract shall be executed by the Member Secretary, or authorized officer MPCB having jurisdiction or the area under his control. The term and condition shall be governed as per the tender document. The Member Secretary of MPCB or any person authorized by him shall be the **ultimate consignee**.

Equipment List

Schedule No.	Brief Description	Qty. ii nos.
1	Continuous Automatic Air Quality Monitoring	1 uni
	Analysers for CO, SO ₂ , NO-NO ₂ -NOx, O ₃ and	each
	Beta Gauge PM2.5 and PM10 Monitors	
2.	BTX Monitor/ Analyser	1 Unit
3.	Multi-calibration systems for gaseous monitors Comprising of gas generation and automated calibration	1 Unit
4.	Sensor based single instrument to measure Meteorological parameters comprising Wind Direction, Wind Speed, Ambient Temperature, Relative Humidity, Solar Radiation and Rainfall mounted on telescoping crank up meteorological Mast	1 Set
5.	Computer system consisting of one PC along with Laser Printer and DAS at the monitoring station and One PC at central office with peripherals and software for data acquisition / Data display Board /transfer and system integration, telephone, Modem.	1 Lot
6.	Modem	2 Units
7.	Arrangements like Thermally Stable Housing (Body Built up on chassis) for installation of Continuous Ambient air quality Monitoring analysers with Sampling line, Internal fitting, Instruments racks, Electrical and Gas line Fittings, Tools (electrical and mechanical).	1 Unit
8.	Split Air Conditioner (2 Ton capacity)	2 Nos.
9.	Petrol Generator set-6.5 KVA	1 No.
10.	Stabilizer-5 KVA	1 No.
11.	Vehicle model number TATA LPT 709Ex 2 or its equivalent, BS-VI variant along with vehicle frame (Chassis build up) air conditioned and thermally stable instrument cabin.	1 No.

Annexure 2

STATION PROTOCOL FOR M UNDER O&M CONTRACT

NAME OF MCAAQMV location:

DATE:

S. No.	Parameter	Status	Zero	o Value		Zero Offset	Spai	n Calik	oration		actor pan)	Rem
			Pre	Post	Pre	Post	Span Sourc	Pre	Post	Pre	Post	
1.	CO Analyzer											
2.	SO2 Analyzer											1
3.	NOx Analyzer											
	NO											
	NO2											
	NOx											
	O ₃											1
4.	BTX Analyzer											
	Benzene					I						
	Toluene											
	E-benzene											
	M+P Xylene											
	O-Xylene											
6.	Dust Analyzer											
	PM2.5											
	PM10											
7.	Meteorological Parameter											
	Temperature											
	Humidity											
	Wind Speed											
	Wind Direction											
	Solar Radiation											
	Rain Fall											
8.	Computers											
9.	ACs and Others											
	Maintenance Detai Requirement	ils/										
	1.											
	Specific Observation(s)											

Station Maintained By..... Station supervised by

DAILY REPORTING FORMAT FOR METREOLOGICAL PARAMETERS

(To be submitted daily at 12 Noon for the previous day ending 12 midnight)

Location:

Date:

Hrs.	WIND SCREEN	WIND DIRECTION	HUMIDITY	TEMPERATURE	SOLAR RADIATION	RAINFALL	REMARKS
00-01							
01-02							
02-03							
03-04							
04-05							
05-06							
06-07							
07-08							
08-09							
09-10							
10-11							
11-12							
12-13							
13-14							
14-15							
15-16							
16-17							
17-18							
18-19							
19-20							
20-21							
21-22							
22-23							
23-24							
Min.							
Max.							
Averag							

MONTHLY REPORTING FORMAT FOR METREOLOGICAL PARAMETERS

(To be submitted monthly next day ending month)

Location: Month:

DATE	WIND SPEED	WIND DIRECTION	HUMIDITY	TEMPERATURE	SOLAR RADIATION	RAINFALL	REMARKS
N # 2							
Min. Max.							
Max. Average							

DAILY REPORTING FORMAT FOR MAIN POLLUTANTS


(To be submitted daily at 12 Noon for the previous day ending 12 midnight)

AMBIENT AIR QUALITY DATA

Location:

Date:

Hrs.	SO ₂	NO	NO ₂	NOX	O ₃	СО	PM _{2.5}	PM 10	C ₆ H ₆	Toluene Xylene	Remarks
00-01											
01-02											
02-03											
03-04											
04-05											
05-06											
06-07											
07-08											
08-09											
09-10											
10-11											
11-12											
12-13											
13-14											
14-15											
15-16											
16-17											
17-18											
18-19											
19-20											
20-21											
21-22											
22-23											
23-24											
Standard											
Min.											
Max.											
Average											

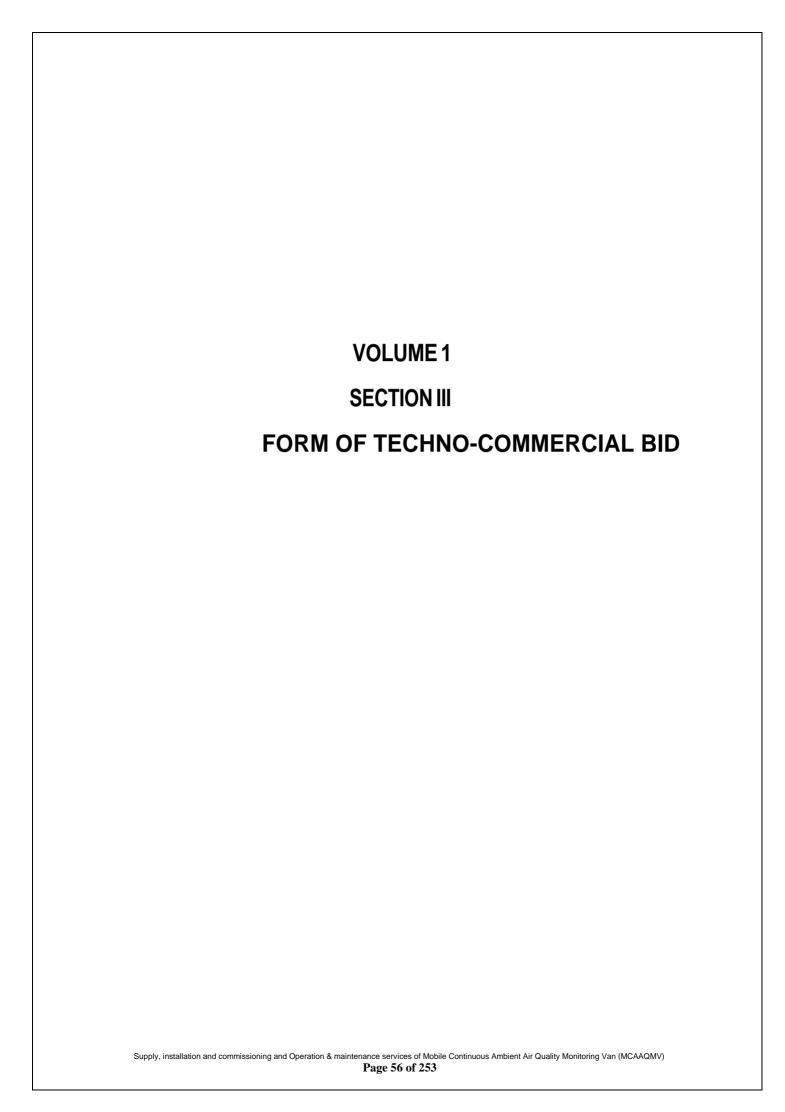

SECTION III

FORM OF TECHNO-COMMERCIAL BID

Number	CONTENTS Page n	0.
Attachment 1	Form of Questionnaire	64
Attachment 2	Certificate of O&M Partner of the Bidder in India	65 to 66
Attachment 3	Form of Letter of Authority	67 to 68
Attachment 3A	Form of Certificate of Supply of Spares and Consumable	es
	By Manufacture	69
Attachment 4	Form of Certificate of Country of Origin	70
Attachment 5	Form of Certificate of Carrying out O&M of CAAQM's By the O&M Partner in India	71
Attachment 6	Form of Equipment List	72
Attachment 7	Form of Manufacturers List	73
Attachment-8A	Proforma for Final Capability for Bidder	74
Attachment 8B	Proforma for Performance Statement for Manufacturer	75
Attachment 8C	Proforma for Performance Statement for Authorized Representative of the Manufacturer	76
Attachment 9	Capability & Experience of O&M Partner	77
Attachment10	Form of Bank Guarantee for Bid Security	78 to79
Attachment11	Form for Pre-requisites for Installation of equipment	80
Attachment12	Deviation Schedule	81
Attachment 13	Indemnity Bond for Handing Over Mobile Continuous	
	Ambient Air Quality Monitoring Van Including All	
	Equipment to the O&M Contractor	82 to 84
Attachment 14	Scheduled Commercial banks (Bid Security)	85
Attachment 15	Scheduled Commercial Banks (Performance Security)	86

<Letterhead of the Bidder>

FORM OF QUESTIONNAIRE

MAHARASHTRA POLLUTION CONTROL BOARD PROJECT

BIDDING DOCUMENTS

SUPPLY, INSTALLATION AND COMMISSIONING AND OPERATION & MAINTENANCE SERVICES OF MOBILE CONTINUOUS AMBIENT AIR QUALITY MONITORING VAN (MCAAQMV)

Date:

To,

The Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, opp. Cine Planet, Near Sion Circle, Sion (East), Mumbai – 400 022.

From: Name of Bidder

Address

Name of Representative

Position

Fax No. Email id.

Signature

Question

Brief report of experience and capabilities and company profile.

<Letterhead of the Bidder>

CERTIFICATE OF O&M PARTNER OF THE BIDDER IN INDIA

To.

The Member Secretary,
Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, opp. Cine
Planet, Near Sion Circle, Sion (East), Mumbai – 400 022.

Subject :-Certificate of Existence of Local Branch, Sales Residential and Representative Office(s) in India

- 1. Name of Office (s):
- 2. Address

Tel. No. : Fax No. : Telex No. : Email id :

- 3. Status of Office(s):
- 4. Date of Establishment of Office (s):
- 5. Name & Address of Residential Representative:
- 6. Total No. of years of association with OEM (Name of the manufacturer):
- 7. Total Manpower:
- 8. Total No. of trained Service Engineer:
- 9. Present No. of offices in India (Name the locations & address):
- 10. Total Turnover in last 3 years:
- 11. Major job in Hand:

Experience in O&M contract: 12.

SI. No.	Name of Client and Address, Phone No. etc.	Description of Contract (Brief scope of contract)	Year of Placement of Order	Present Status

Signature		
Name:		
Designation:		
Seal:		

FORM OF LETTER OF AUTHORITY

To,

The Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, opp. Cine Planet, Near Sion Circle, Sion (East), Mumbai – 400 022.

Name of Manufacturer

Subject: -Letter of Authority from Manufacturer

Dear Sirs,

We, (Name of Manufacturer), a manufacturer duly organized and existing under the law of (Country Name) with its principal office of business as (Address) hereby make, constitute and appoint (name of Bidder), a company duly organized and existing under the laws of (Country Name) with its principal office of business at (Address) to be our true and lawful attorney in fact to do the following sets and deeds:

To present and bind us in the for Supply, Installation And Commissioning And Operation & Maintenance Services Of Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV) for MAHARASHTRA POLLUTION CONTROL BOARD at in the State of India, regarding the Supply and installation of the following equipment proposed in the bid which we manufacture or produce.

Item No.	Name of Equipment

We, as a manufacturer bind ourselves as co-worker of the bid and are jointly and severally responsible for the compliance of the said bid and once (Name of Bidder) has been selected as a successful bidder, we shall manufacture, delivery and install the equipment in accordance with the terms and conditions of contract with (Name of Bidder) and the State Pollution Control Board.

IN WITNESS WHEREOF, we have hereto signe	ed this document on
ACCEPTED ON, 2021	
NAMEOFBIDDER MANUFACTURER	NAME OF ISSUING AUTHORITY
(Name of duly authorized Representative to sign and signature)	(Name of duly authorized representative to sign and Signature)
(Rank of position and department)	(Rank of position and department)

Attachment 3A

Date:

To.

Name of Manufacturer:

Office Seal of Manufacturer: Legal Address of Manufacturer:

•							
The Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, opp. Cine Planet, Near Sion Circle, Sion (East), Mumbai – 400 022.							
Sub:-Certificate o	Sub:-Certificate of SUPPLY of Consumables and Spare Parts by Manufacturer						
parts of the equip detail) to the cont It is hereby guara the following equ	This is to certify that we (Name of Manufacturer) shall SUPPLY the consumables and spare parts of the equipment mentioned below during O&M period under the contract (contract detail) to the contractor (Name of the contractor)/ Owner. It is hereby guaranteed that we shall maintain stocks of consumables and spare parts for the following equipment for a period of Eight (8) years after the commissioning of the equipment in India.						
Item No.	Name of Equipment	Name of Manufacturer					
Signature: Name of Pers Position:	on:						

<Letterhead of the Manufacturer> FORM OF CERTIFICATE OF COUNTRY OF ORIGIN

To,

The Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, Cine Planet, Near Sion Circle, Sion (East), Mumbai – 400 022.

Name of Manufacturer

Subject:-Certificate of Country of Origin

We, (Name of Manufacturer), hereby certify that our equipment for procurement and installation of equipment for Maharashtra Pollution Control Board in the State of, India is to be manufactured in the country mentioned below:

Item No.	Name of Equipment	Country of Origin

S	Si	g	r	16	۱	tι	I	r	е	,

Name of Person:

Title:

Name of Manufacturer:

Legal Address:

<Letterhead of the O&M Partner>

FORM OF CERTIFICATE OF CARRYING OUT O&M OF MCAAQMV'S BY THE O&M PARTNER IN INDIA

Date:

To.

The Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, opp. Cine Planet, Near Sion Circle, Sion (East), Mumbai – 400 022.

Sub:-Certificate of carrying out O&M of MCAAQMV's by the O&M partner in India.

This is to certify that we <Name of O&M Partner> hereby agree to carry out day to day Operation and maintenance of the one (1) MCAAQMV installed and commissioned by <Name of the main bidder> for minimum of five years from the date of installation & commissioning of the MCAAQMV at the rates quoted by <Name of the main bidder>against this tender, strictly in accordance with terms & conditions contained in this bid document.

Signature:

Name of Person:

Position:

Name of O&M Partner:

Name Seal of O&M Partner:

Legal Address of O&M Partner in India:

Counter-signed by main bidder Name

of Person:

Position:

Name of the Bidder:

Office Seal of Bidder:

Legal Address of Bidder:

<Letterhead of the O&M Partner> LIST of Equipment Imported and indigenous

S. No.	Name of equipment	Name of manufacturer Quantity				

<Letterhead of the O&M Partner> LIST of Manufacturer Imported and indigenous

S. No.	Name of equipment	Name of manufacture

Attachment 8 A

PROFORMA FOR FINANCIAL CAPABILITY OF BIDDER (for a period of last three years)

Bid	No.	Package	Code	Date	of	Opening	
Time		***************************************					
Nam	e of th	e Bidder					

Year	Currency	Turnover
2018-2019 financial year		
2019-2020 financial year		
2020-2021 financial year		
Average		

Note:

- 1. The annual turnover amount is to be supported by annual report.
- 2. Financial Capability: The Minimum required annual turnover in respect of Procurement of Supply Installation and commissioning of goods for the successful bidder in the last Three (3) years shall be of amount of RS. 60 Cr. Minimum annually.
- 3. Enclose supporting document such as audited balance sheet/CA Certificate.

Signature of the Authorized Representative Name of the Person Position

Attachment 8 B

PROFORMA FOR PERFORMANCE STATEMENT FOR MANUFACTURER (for a period of last five years)

Bid NoName of Equipment_			Date of Opening					
		Time						
Name	Name of the Manufacturer							
	Order	Description	Quantity	Value	Date of	Has the equipment		
/	No. &	of	supplied	of	commissioning	been satisfactory		
000	Data	ordered		ordor	and	Functioning?		

Order	Order	Description	Quantity	Value	Date of	Has the equipment
placed by	No. &	of	supplied	of	commissioning	been satisfactory
(full address	Date	ordered		order	and	Functioning?
of		equipment			handing	(Attach certificates
Purchaser)		(Model			over	from the Purchaser/
		no.)				Consignee for each
						equipment)
1	2	3	4	5	6	7

NOTE: Bidder to furnish above detail for each equipment of the quoted package on separate sheet.

Signature of the Authorized Representative Name of the Person Position

Attachment 8 C

PROFORMAFOR PERFORMANCE STATEMENT FOR BIDDER (O&MOPERATOR) AS AUTHORIZED REPRESENTATIVE OF THE MANUFACTURER (for a period of last five years)

Bid No	_ Name of Equipment	Date of Opening
	Time	
Name of the	Manufacturer	

Order placed by (full address of Purchaser)	Order No. & Date	Description of ordered equipment (Model no.)	Quantity supplied	Value of order	Date of Commission in g and handing over	Has the equipment been satisfactory Functioning. (Attach certificates from the Purchaser/ Consignee for each equipment)
1	2	3	4	5	6	7

NOTE: Bidder to furnish above detail for each equipment of the quoted package on separate sheet.

Signature of the Authorized Representative Name of the Person Position

CAPABILITY & EXPERIENCE OF O&M PARTNER

Name and address of the O & M Partner in India (if applicable):

SI. No.	Name of the O&M Personnel proposed to be deployed	Educational Qualification	Experience in no. of years in carrying out O&M of	Detail curriculum Vitae Attached
1.			MCAAQMV.	(YES / NO)
2.				
3.				
4.				
5.				
6.				
7.				
8.				
9.				

FORM OF BANK GUARANTEE FOR BID SECURITY

(To be stamped in accordance with Stamp Act, if any, of the Country of the issuing Bank)
Bank Guarantee No
Ref. No.:-
To,
The Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3 rd Floor, opp. Cine Planet, Near Sion Circle, Sion (East), Mumbai – 400 022.
Dear Sirs,
WHEREAS (hereinafter called "the Bidder") has submitted its bid dated for Supply, Installation And Commissioning And Operation & Maintenance Services Of Mobile Continuous Ambient Air Quality Monitoring Var (MCAAQMV) for MAHARASHTRA POLLUTION CONTROL BOARD at Mumba (hereinafter called "The Bid")
KNOW ALL MEN by these present that WE of having our registered office at (hereinafter called "The Bank") are bound unto MAHARASHTRA POLLUTION CONTROL BOARD, India (hereinafter called "The Board") in the sum of(amount as per bid document in Indian Rs. Or US \$, both in words and figures), for which payment well and assign, by these presents. Sealed with the common seal of the bank this day
THE CONDITIONS of this obligation are:
If a Bidder withdraws / modifies its Bid during the period of Bid validity specified in Sub-

clause 4.6 hereunder;

Or

- 2. If the bidder having been notified of the acceptance of its bids by the Board during the period of bid validity:
 - a. fails or refuses to execute the Contract Form, when requested; or
 - b. fails or refuses to furnish the Performance Security, in accordance with the Instruction to Bidders.

Or

3.	In case bidder refuses to withdraw, without a which the bidder did not state in the Deviation	· ·
	upon receipt of, its first written demand, v demand, provide that in its demand the	the above amount, according to, and without the Board having to substantiate its Board will note that the amount claimed of one or all of the three above stated dition or conditions.
		[NAME OF BANK]
		By(Title)
		Authorized Representative
	(Signature of Witness)	
Nam	ne of Witness	
Add	ress of Witness	

PRE-REQUISITES FOR INSTALLATION OF EQUIPMENT

To,

The Member Secretary,
Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, opp. Cine
Planet, Near Sion Circle, Sion (East),
Mumbai – 400 022

Dear Sir,

Following are the pre-requisites for installations of the equipment offered by us, which are required to be provided by you prior installation of the equipment:

Package no. / Item No.	Name of the Equipment	Installation & commissioning pre- requisites*

Signature of the Authorized Representative Name of the Person Position

Note:

SUPPLY, INSTALLATION AND COMMISSIONING AND OPERATION & MAINTENANCE SERVICES OF MOBILE CONTINUOUS AMBIENT AIR QUALITY MONITORING VAN (MCAAQMV) AT -----FOR MPCB

(Deviation Schedule)

Bidders Name & Address

To,

The Member Secretary,
Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, opp. Cine
Planet, Near Sion Circle, Sion (East),
Mumbai – 400 022

Dear Sir,

Subject:- Deviation Schedule.

We declare that the following are the only and exhaustive deviations, variations from, exceptions and exclusions to the Bidding Documents for Services as outlined in your Technical Specifications for the subject package. Except these deviations, subject to the approval and acceptance by you, the entire work shall be performed as per your specifications and documents. Further, we agree the additional conditions, if any found elsewhere in the offer other than those stated below, save that pertaining to any rebates / discount offered, shall not be given effect to:

Equipment Code No.	Vol./Clause Ref./ Page No.	As Specified in the Documents	Bid	Deviation and Variations to the Bid document

Date:	(Signature)
Place	(Printed Name)
	(Designation)
	(Common Seal)

INDEMNITY BOND FOR HANDING OVER MOBILE CONTINUOUS AMBIENT AIR QUALITY MONITORING VANSINCLUDING ALL EQUIPMENT TO THE O&M CONTRACTOR

This I	demnity Bond is made this Day of 2021 By	.a
	iny registered under the CompanieAct,1956/Partnership firm / Proprietary concern havir stered office at(hereinafter called as "Contractor" o "obligator" which expression shall include i	r
BOAF	sors and permitted as signs)in favour of MAHARASHTRA POLLUTION CONTRO D with Office at Mumbai, which term shall include permitted assigns and successor after called "MPCB" which expression shall include its successors and assigns).	L
one n No which	as MPCB has awarded to the Contractor, a contract for O&M of the . Mobile Continuous Ambient Air Quality Monitoring Vans (MCAAQMV) located at –, vide its Letter of Intent /Award Letter /Contract dated	
Now,	nerefore this Indemnity Bond witnessed as follows:	
	That in consideration of various Equipments as mentioned in the Contract, valued at Rs	ne
2.	that the Contractor is obliged and shall remain absolutely responsible for the safe custor of the Equipments at Mobile Continuous Ambient Air Quality Monitoring Var MCAAQMV) belonging to MPCB against all risk whatsoever till the Equipments are duly used in accordance with all term of the Contract. The Contractor undertakes to keep MPCB harmless against are seen of the Contract.	ns KS ns
	The Contractor undertakes that the Equipments shall be used exclusively or the performance/ execution of the Contract strictly in accordance wis terms and conditions and no part of the Equipments shall be utilized for ny other work or purpose whatsoever. It is clearly understood by the Contractor that non-observance of the obligations under this Indemnity Borly the Contractor shall inter-alia constitute a applicable law breach of trust on the past of the Contractor for all intents and purposes including legal / penal consequences.	or ne nd art

That MPCB is and shall remain the exclusive Owner of the Equipment free from all encumbrances, charges or liens of any kind, whatsoever. The

4.

Equipments shall at all times be open to inspection and checking by Project-in-Charge MPCB shall always be free at all time to take possession of the Equipments in whatever form the equipments may be. If in its opinion, the equipments are likely to be endangered, misutilised or converted to uses other than those specified in the Contract, by any act of omission or commission on the part of the Contractor; he finds itself and undertakes to comply with the direction or demand of MPCB to return the Equipments without any demur or reservation.

- 5. That this Indemnity Bond is irrevocable. If at any time any loss or damage occurs to the Equipments or the same or any part thereof is misutilised in any manner whatsoever then the Contractor hereby agrees that the decision of the Project-in-Charge of MPCB as to assessment of loss or damage to the Equipments shall be final and binding on the Contractor. The Contractor binds itself and undertakes to replace the lost and / or damaged Equipments at its own or remedy that may be available to MPCB against the Contractor under the Contract and under this Indemnity Bond.
- 6 Now the condition of this Bond is that if the Contractor shall duly and punctually complies with the terms and conditions of this bond to the satisfaction of MPCB, then the above bond shall be void, but otherwise, it shall remain in full force and virtue.

In witness whereof, the Contractor has here un to set its hand through its authorized representative under the common seal of the company, the day month and year first above mentioned.

SCHEDULE NO. 1

Particulars of the	Quantity	Value of the	Signature of
Equipments		Equipment	Authorised Person
handed over			

		For and on behalf of M/s
Witnes	s I	
1.	Signature	
2.	Name	
3.	Address	Name Signature Designation Authorized representative
Witnes	s II	
1.	Signature	
2.	Name	

3.

Address

(Common Seal)

(In case of Company)

LIST OF BANKS ACCEPTABLE FOR SUBMISSION OF BANK GUARANTEE FOR BID SECURITY

LIST OF BANKS

(A) SBI AND ASSOCIATES

- 1. State Bank of India
- 2. State Bank of Bikaner and Jaipur
- 3. State Bank of Hyderabad
- 4. State Bank of Indore
- 5. State Bank of Mysore
- 6. State Bank of Patiala
- 7. State Bank of Saurashtra
- 8. State Bank of Travancore

(B) NATIONALISED BANKS

- 1. Allahabad Bank
- 2. Andhra Bank
- 3. Bank of India
- 4. Bank of Maharashtra
- 5. Canara Bank
- 6. Central Bank of India
- 7. Corporation Bank
- 8. Dena Bank
- 9. Indian Bank
- 10. Indian Overseas Bank
- 11 .Oriental Bank of Commerce
- 12. Punjab National Bank
- 13. Syndicate Bank
- 14 .Union Bank of India
- 15 .United Bank of India
- 16. UCO Bank
- 17. Vijaya Bank
- 18. Bank of Baroda

LISTOFBANKS ACCEPTABLE FOR SUBMISSION OF BANKGUARANTEES FOR ADVANCE PAYMENTS, PERFORMANCE SECURITIES AND SECURITIES FOR DEED OF JOINT UNDERTAKING

LIST OF BANKS A.SBI and Associates

- 1. State Bank of India
- 2. State Bank of Bikaner and Jaipur
- 3. State Bank of Hyderabad
- 4. State Bank of Indore
- 5. State Bank of Mysore
- 6. State Bank of Patiala
- 7. State Bank of Saurashtra
- 8. State Bank of Travancore

B. Nationalised Banks

- 1. Allahabad Bank
- 2. Andhra Bank
- 3. Bank of India
- 4. Bank of Maharashtra
- 5. Canara Bank
- 6. Central Bank of India
- 7. Corporation Bank
- 8. Dena Bank
- 9. Indian Bank
- 10. Indian Overseas Bank
- 11. Oriental Bank of Commerce
- 12. Punjab National Bank
- 13. Syndicate Bank
- 14. Union Bank of India
- 15. United Bank of India
- 16. UCO Bank
- 17. Vijaya Bank
- 18. Bank of Baroda

VOLUME I	
SECTIONIV	
FORM OF FINANCIAL BID	
(Online Submission only)	
Supply, installation and commissioning and Operation & maintenance services of Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV) Page 81 of 253	

SECTION IV

FORM OF FINANCIAL BID

Sr.no.	CONTENTS	Page number
Attachment	1 Bid Form	89 to 90
Attachment 2	Summary of Bid Price	92 Attachment
3 Bid Price	Breakup Equipment of Foreign Origin (CIF Price)93 Attac	hment 3A Bid
Price Breakup	For O&M of MCAAQMV's for Five Year	94

<Letterhead of the Bidder>

Date:	
Grant	no.:
Bid No.	

BID FORM

(Must be Submitted Scan Copy Online)

(Selected bidder will be submitted original Letter after receiving LOA for this office record)

To,

The Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, opp. CinePlanet, Near Sion Circle, Sion (East), Mumbai – 400 022

Gentlemen:

- 1 Having examined the Bidding documents for procurement, installation & commissioning and Operation & Maintenance of MCAAQMV's at -----(number(s)) locations, MPCB (herein after referred to as "the Works"), including, but not limited to, the Instructions to Bidders, Scope of Works, General and Special Conditions of Contract, Technical Specifications, Schedules, Attachments, Amendment Nos. we, the undersigned, offer to execute and complete the whole of the works and remedy any defects therein, in conformity with the said Bidding Documents for the sum of International trading currency (in figures.....) for the equipment including all other charges as mentioned in the document, supplied from Foreign Origin and Indian Rupees...... (INR......) for the incidental costs incurred in India (if any) as may be ascertained in accordance with the Summary of Bid Price and Bid Price breakup attached herewith and made part of this bid.
- We undertake, if out Bid is accepted, to complete and deliver the wholeof the Works comprised in the Contract within the time specified in the contract, subject

to the said conditions. 3. If our Bid is accepted, we will obtain the guarantee of a bank in a sum Equivalent to -----percent of the Contract Price for the due performance of the Contract, in the form prescribed by the Board. 4. We agree to abide by this Bid for a period of One hundred eighty (180) days from the final date of the submission of Bid fixed in sub-clause 7.2 of the Instruction of Bidders, and shall remain biding upon us and may be accepted at time before the expiration of that period. anv 5. Unless and until a formal Contract is prepared and executed, this Bid, to get herewith your written acceptance thereof, shall constitute a binding Contract between us. 6. We understand that you are not bound to accept the lowest of any bid you may receive, and that you will not defray any expense incurred by us in bidding. Date this day of 2021. Signature ____in the capacity of _____ Duly authorized to sign Bid for and on behalf of -----(IN BLOCK CAPITAL) Address Facsimile number Telephone Number **Email** id. **WITNESS** Address

Occupation _____

SUMMARY OF BID PRICE

DESCRIP	PTION	TOTAL VALUE	
I. SUPPL	YOF THE EQUIPMENT		
1) For go	ods supplied from abroad (In Bid-Currency)		
a.	FOB price for Package		
b.	Freight		
C.	Insurance up to port of de-embarkment		
CIF Price	at port of de-embarkment (bid currency) (1a + 1b + 1c)		
2) Local	Costs for goods supplied from abroad		
a.	Port handling and clearance charges.		
b.	Transportation cost from Port of de-embarkment to Sites		
C.	Insurance from Port of de-embarkment up to handing		
over			
d.	Installation and commissioning		
S	ub-total (2a + 2b + 2c + 2d)		
3) For the	e Goods Supplied from India		
a.	The price of the Equipment quoted ex-works, ex-factory,		
	ex-warehouse, ex-showroom, or off-the-shelf including all		
	customs duties and sales and other taxes already paid or		
	payable on the components and raw material used in		
	the manufacture or assembly of the Equipment quoted		
	ex-works or ex-factory.		
b.	Price for handling and inland transportation, insurance		
	up to handing over the equipment at Site and other		
	local costs upto delivery of the Equipment to each Site.		
C.	Installation and commissioning		
d.	Price of other incidental cost, if any. Then the Bidder		
	shall specify the same.		
e.	The price of Vehicle model number TATA LPT 709Ex 2 or its		
	equivalent, BS-VI variant along with vehicle frame (Chassis build up)		
	air conditioned and thermally stable instrument cabin.		
Sub-tota	I (3a + 3b + 3c + 3d+3e)		
4) Other	incidental costs, if any (such as Indian agents		
	sion) in INR		
TOTAL F	FOR SUPPLY (1 + 2 + 3 + 4)		
	0&M cost for five years for analyser systems as indicated in		
Attachme	ent 3A		
III Total (O&M cost for five years for Mobile Vehicle as indicated in		
Attachment 3B			
IV.COST	OF TRAINING(bid currency)		
GRAND '	TOTAL CONTRACT PRICE (BID CURRENCY/INR) (I + II + III)		

- **NOTE:** 1. ALL LOCAL TAXES, DUTIES& LEVIES ARE PAYABLE AT ACTUAL (EXTRA) BY THEOWNER (MPCB).
 - 2. QUOTED COST OF O&M OF A MCAAQMV FOR EACH YEARSHOULD BE AT LEAST 12% OF THE COST OF SUPPLY& INSTALLATION OF THE MCAAQMV.IN CASE THE BIDDER QUOTES O&M COST LOWER THAN 12% OF THE SUPPLY&INSTALLATION COST, THE OWNER WILL REDUCE THE SUPPLY&INSTALLATION COST SUITABLY, SO AS TO MAKE THE O&M COST AS 12% OF SUCH SUPPLY&INSTALLATION COST, KEEPING THE TOTAL QUOTED COST AS UNCHANGED.
 - 3. INDIAN AGENT'S COMMISSION SHALL BEPAID IN INDIAN RUPEES ONLY. MARKET EXCHANGE RATE RULING ON THE DATE OF AWARD IN ACCORDANCE WITH CLAUSE 4.3 (b) OF INSTRUCTIONS TO BIDDER (SECTION-I) WILL BE APPLICABLE FOR THIS PURPOSE.
 - 4. O & M COST SHALL BE QUOTED AS INDICATED IN ATTACHMENT 3A.

BID PRICE BREAKUP FOR EQUIPMENT (CIF) PRICE

S. No.	Item / Analyzer Name	Quantity in Nos. / Sets	Unit Price (BID CURRENCY)	TOTAL Price (BID CURRENCY)
1.	Automatic Ambient CO Analyzer			
2.	Automatic Ambient SO ₂ Analyzer			
3.	Automatic Ambient NO-NO ₂ -NOx Analyzer			
4.	Automatic Ambient O ₃ Analyzer			
5.	PM ₁₀ Monitor			
6.	PM _{2.5} Monitor			
7.	BTX Analyzer			
8.	Multi-calibration systems for gaseous monitors comprising of gas SUPPLY/ generation and automated calibration			
9.	Sensor Based Meteorological Instrumentation comprising Wind direction, Wind speed, Ambient temperature, Relative humidity, Solar Radiation and Rainfall mounted on telescoping crank up meteorological Mast.			
10	Computer system consisting of one PC along with Laser Printer and DAS at the monitoring station and one PC at central office with peripherals and software for data acquisition / Data display Board / transfer and system integration, telephone, Modem.			
11	Arrangements like Thermally Stable Housing (Body Built up) for installation of Continuous Ambient air quality Monitoring analysers with Sampling line, Internal fitting, Instruments racks, Electrical and Gas line Fittings, Tools (electrical and mechanical).			
12	2 Ton capacity split Air conditioner			
13	Petrol Generator set-6.5 KVA			
14	Stabilizer- 5 KVA			
15	Vehicle model number TATA LPT 709Ex 2 or its equivalent, BS-VI variant along with vehicle frame (Chassis build up) air conditioned and thermally stable instrument cabin.			

Attachment 3A BID PRICE BREAKUP FOR O&M OF MCAAQMV (Analyser Systems) FOR FIVE YEARS


SI. No.	Year of O&M	O & M Cost/Van including Cost of (Incidental Charges consisting of security, Electricity, Phones/ internet, Manpower, AMCs material including spares & consumables for Operation & maintenance and other in Rs	Qty. of MCAAQMV	Total O & MCharges for the year in Rs.	
1.	1 st year				
2.	2 nd year				
3.	3 rd year				
4.	4 th year				
5.	5 th year				
TOTAL					

NOTE: TAXES APPLICABLE SHOULD BE MENTIONED SEPARATLY.

Attachment 3B BID PRICE BREAKUP FOR O&M OF MOBILE VEHICLE FOR FIVE YEARS

SI. No.	Year of O&M	Vehicle Cost of S Operation Maintenal vehicle chassis. a the This achieved laid-out	nce of the	Qty. of MCAAQMV		Total O & MCharges for the year in Rs.	
1.	1 st year						
2.	2 nd year						
3.	3 rd year						
4.	4 th year						
5.	5 th year						
TOTAL	1						

NOTE: TAXES APPLICABLE SHOULD BE MENTIONED SEPARATLY.

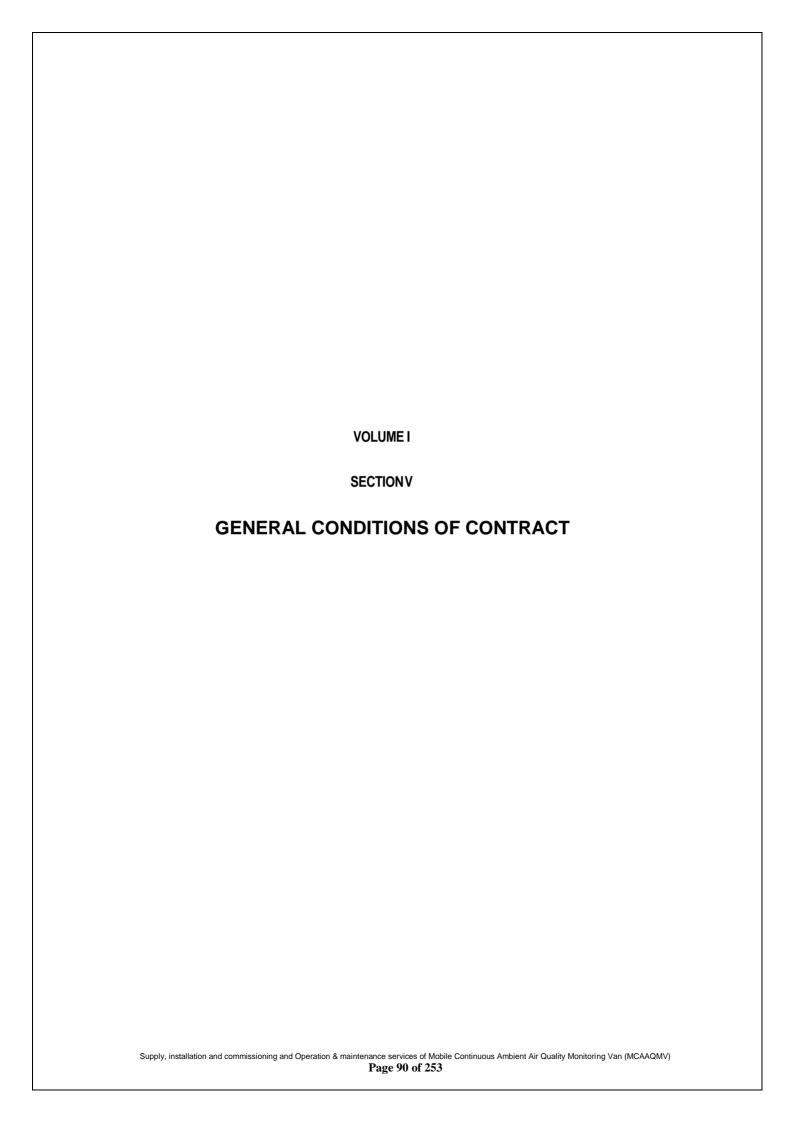

SECTION V

Sr. No	. GENERAL CONDITION OF CONTRACT CONTENTS	Page number
1.	Definitions	92
2.	Intent of Contract	93
3.	Performance of Works	93
4.	Use of Contract Documents and Information	93-94
5.	Location	94
6.	Language and Calendar	94
7.	Site Condition	94
8.	Country of Origin	94
9.	Specification of Equipment	95
10.	Code and Standard	95
11.	Electrical Ratings	96
12.	Name Plate	96
13.	Packing & Marketing	97
14.	Shipment	97
15.	Protection and Safety	98
16.	Work Schedule	99
17.	Projection Formation	99
18.	Warranty / O&M Contractor	100
19.	Insurance	100
20.	Installation	100
21.	Inspection and Test	100 to 103
22.	Training	103
23.	Completion	103
24.	Submission of Documents	103
25.	Payment	104
26.	Prices	104
27.	Performance Security	104
28.	Assignment	105
29.	Subcontract	105
30.	Delays in the Contractor's Performance	105
31.	Liquidated Damages	106
32.	Suspension of Work	106
33.	Termination for Default	106
34.	Force Majeure	106
35.	Termination of Insolvency	107
36.	Resolution of Disputes	107
37.	Taxes and Duties	108
38.	Injury and Damage	110
39.	Royalty and Patents	111
40.	Effectiveness	111
41.	Laws and regulations	111
42.	Notices	112

GENERAL CONDITIONS OF CONTRACT

These conditions encompass all the Works to be executed and completed by the Contractor for the Project and as further defined herein.

1.0 DEFINITION

Unless the context of the General and Special Conditions of Contract otherwise requires, the following terms wherever in the General and Special Conditions of Contract shall have the meaning defined hereunder.

Words imparting the singular shall also include the plural and vice versa where the context requires. Whether the words and phrases defined in this Clause are capitalized or not in the Contract shall not affect their meaning.

- 1.1 "The **Project**" or "The Works" means Supply, Installation, Commissioning and Providing O & M Service of MCAAQMV to be installed in the State of Maharashtra- 15 Nos. and their Operation & Maintenance at defined locations under the supervision and control of (**Maharashtra Pollution Control Board**).
- 1.2 "The Contract" means the written agreement to be concluded between the Board and the Contractor and includes terms and conditions stipulated on the Bidding Documents and any other descriptions annexed thereto which form an integral part of the agreement to be provided by the Board.
- **1.3** "The **Contract Price**" means the price payable to the Contractor under the Contract for the full and proper performance of its contractual obligations for the Works.
- **1.4** "The **Equipment**" means all kind of materials, Machinery, Components, apparatus, articles and instruments for the Project to be provided by the Contractor to the, Board under the Contract.
- **1.5** "GCC" means the General Conditions of Contract contained in this Section.
- **1.6 "SCC"** means the Special Conditions of Contract in Section VI of this Volume.
- 1.7 "S/W" means the Scope of Works in Section II of this Volume.
- 1.8 "The **Contractor**" means the firm SUPPLY the Equipment and-performing the Works in connection with the Project under the Contract and includes his personal representatives, successors and authorized assignees.
- 1.9 The "Manufacturers" means the firms, which produce the Equipment to be furnished by the Contractor under the Contract with the Board.
- 1.10 "The **Specifications**" means the specifications of the Works to be

performed by the Contractor in conformity with those specified in both the Technical Specifications of Volume II and all other related documents in the Bidding Documents, and modifications thereof or additions thereto as may from time to time be made, and approved in writing by the Board in case of prior to the Contract and agreed upon by both the Board and the Contractor after the Contract.

1.11 "The **Sites**" means MCAAQMV's to be installed as specified in Clause 1 of Scope of Works (Section - II).

2.0 INTENT OF CONTRACT

- 2.1 The intent and spirit of the Contract is to provide all the details for the Works herein specified to be fully completed within the duration of the Contract.
- 2.2 It is hereby understood that the Contractor, in accepting the Contract, agrees to furnish any and everything necessary for such intent notwithstanding any omission in the Contract.

All matters omitted from the Contract which may reasonably be inferred to be obviously necessary for the efficient and stable completion of the Works shall be deemed to be included in the Contract and the Contractor shall be held responsible for any errors or losses which the Contractor may make due to such omissions as above.

3.0 PERFORMANCE OF WORKS

Unless otherwise provided for, the Works shall be performed by the Contractor in compliance with S/W, GCC, SCC and the Specifications in this Bidding Documents issued by the Board and Contract to be concluded between the Board and the Contractor.

Unless otherwise agreed or stated, the Contractor shall bear all the cost and take all the responsibilities for the performance of all the Works.

4.0 USE OF CONTRACT DOCUMENTS AND INFORMATION

- 4.1 The Contractor shall not, without the Board's prior written consent, disclose the Contract, or any provision thereof, or any specification, plan, drawing, pattern, sample, or information furnished by or on behalf of the Board and their authorized personnel and body in connection therewith, to any person other than a person employed by the Contractor in the performance of the Contract. Disclosure to any such employed person shall be made in confidence and shall extend only so far as may be necessary for purposes of such performance.
- **4.2** The Contractor shall not, without the Board's prior written consent, make use of any documents or information enumerated here above except

for purposes of performing the Contract.

4.3 Any documents other than the Contract itself, enumerated in here above shall remain the property of the Board and shall be returned to the Board on completion of the Contractor's performance under the Contract if so required by the Board.

5.0 LOCATION

As defined by the Board as per list attached at IFB.

6.0 LANGUAGE AND CALENDAR

6.1 Language

All documents and correspondence related to the Contract shall be made in English.

6.2 Calendar

All dates, months, years and terms referred in the Contract shall relate with the Gregorian Calendar, unless otherwise mentioned specifically.

7.0 SITE:

The location sites of the MCAAQMV would be primarily at the Regional Offices and as per the list depicted on page 17 of this document.

8.0 COUNTRY OF ORIGIN

- **8.1** All the Equipment supplied under the Contract shall have their origin in the eligible countries.
- 8.2 For the purposes of this Clause, "Origin" means the place where the Equipment were produced manufactured. The Equipment is produced or though manufacturing, processing, or substantial and manufactured when, major assembly of components, a commercially recognized new product results that is substantially different in basic characteristics in purpose or utility from its components.
- **8.3** The origin of Equipment is distinct from the nationality of the Contractor.

9.0 SPECIFICATION OF EQUIPMENT

9.1 Equipment

The Contractor shall Supply all the Equipment specified in the package quoted as per the package wise Equipment List of Attachment 1.. All the Equipment to be supplied under the Contract shall be new and unused.

9.2 Specification of Equipment

The performance, materials, duty, workmanship, operating conditions and design conditions for the Equipment shall meet and comply with the Tender Specifications.

The Specifications indicate the principal and minimum technical requirements for each equipment. The details of the Equipment shall be fully examined and suitably selected through the detailed engineering and design without sacrifice in quality of serviceability of the Equipment.

The figures of dimension and weight shown in the Specifications are indicatively presented as approximate figures. These figures may not necessarily and exactly be applied for the selection of the Equipment, but the Contractors shall meet the principal and minimum requirements shown in the Specifications. Any Bidder offering better specification than the minimum prescribed shall be considered as technically qualified.

10. CODE AND STANDARD

10.1 Code and Standard

All the Equipment and the Works shall conform to the approved and authorized codes and standards of the origin country, the following standards wherever applicable and Indian Standard which are in force at the moment of the installation.

- Japanese Industrial Standard (JIS)
- Environmental Protection Agency of United States (U.S EPA)
 Standard
- International Organization for Standard (ISO)
- British Standard (BS)
- TUV Germany
- MCERTS- SIRA certification U.K Environment Agency

Other internationally prevailing standards are accepted for the Equipment, unless otherwise indicated.

Even if some codes and standards are designated in the Specifications, the other codes and standards not shown therein are also applicable instead of the designated ones as far as they are equivalent to such designated codes and standards and meet the requirement thereof.

10.2 Metric System

All dimensions and performance of the Equipment shall be stated in metric system, unless otherwise specified in the Specifications.

11.0 ELECTRICAL RATINGS

11.1 Electrical Rating

The Equipment shall conform to the following ratings and standards wherever applicable.

- 1) All the electrically operated equipment specified herein shall be single phase, 230 Volts ±10 volts AC and 50 Hz ±3% unless otherwise specified in the Specifications.
- 2) Electrical plugs for the Equipment shall conform to local regulations and standards.

11.2 Precaution against Voltage Fluctuation

Adequate automatic voltage regulator for the Equipment shall be arranged by the Contractor wherever indicated in the Specifications. The Contractor shall pay due attention to that electrical voltage fluctuation exerts a serious influence and damage upon functioning of the equipment.

12.0 NAME PLATE

Nameplate shall be affixed on a suitable place of the Equipment in accordance with the provision of SCC.

13.0 PACKING AND MARKING

13.1 Packing

1) Transportation by air cargo

> The Contractor shall pack and transport the Equipment in the double carton, approved by airline and deliver separately to the designated Site in complete condition.

2) Transportation by vessel

> The Equipment shall be packed and transported for seaworthy shipment in such a manner that they are carried to the Sites in complete condition. The packages shall be made shockproof, waterproof, moisture proof and any other protection against rough handling, exposure precipitation, open storage and other severe tropical temperature. salt, conditions during transit to each final Site. These Equipment shall be transported by container vessel and packed separately for the designated Site.

13.2 Marking

The outside of the package shall be marked in accordance with SCC in such a manner that they are clearly visible, protected against loss and resistance to external influences.

13.3 Packing List

Contents of each package and/or the Equipment shall be itemized on a detailed list showing the exact weight, and extreme outside dimensions of length, width and height of each package and/or the Equipment. One copy of the detailed packing list indicating name of components, assembly number and quantity which corresponds to those of the Equipment in each package shall be enclosed in each package.

Enclosed in one package, there shall also be a master packing list summarizing and identifying each individual package. Packing list shall be placed in a waterproof cover and secured against any external influence of the package.

14.0 SHIPMENT

14.1 Shipment

Shipment of the equipment from foreign origin shall be made as specified in SCC.

14.2 Shipping Documents

Promptly after shipment of equipment of foreign origin, the Contractor shall airmail the shipping documents to the Board in accordance with SCC.

14.3 Unloading and Custom Clearance

The Contractor shall arrange the clearing agent for unloading, customs clearance and storage of the equipment from the Foreign Origin, documentation and all the other procedures.

497

The Board will agree to assist the Contractor where required in obtaining clearance of the Equipment through the customs and provide exemption certificate, if required.

14.4 Inland Transportation

The Contractor shall be fully responsible for the delivery of all the Equipment to the Sites.

The Contractor shall arrange at his option and cost for the transportation from the port of entry to each Site for the equipment of foreign origin.

Transportation of Radioactive material if any shall be carried out by the contractor and contractor will obtain statutory clearances for the same.

14.5 Handling and Storage

The Contractor shall protect the Equipment from any damage and avoid overloading. Particular attention shall be given to the perishable

Equipment and those which must be kept dry, cool or from exposure to direct sunshine and moisture.

In case a part of the Board's facilities is necessary to be occupied by the Contractor for temporary storage or installation use, the Contractor shall obtain the written approval from the Board for temporary occupation and protect facilities against any damages. Charges payable for this facility to the Board for this shall be fixed by the Board.

15.0 PROJECTION AND SAFETY

The Contractor shall be totally responsible for all the reasonable precautions against fire in respect of the Works, temporary works, offices, storage yards and other places and things connected therewith.

The Contractor shall comply with all rules, regulations and orders which have been made by the Government of India, the Board or any other competent authority and the contractor shall provide sufficient fire- fighting protection in respect of the safety of the property and personnel of the Board.

16.0 WORKS SCHEDULE

The time schedule for the Works to be carried out by the Contractor is specified in SCC.

The Contractor shall complete the Works in accordance with the Works schedule specified here above.

17.0 PROJECT FORMATION

17.1 MPC Board

The authorized personnel from Maharashtra Pollution Control Board for the Project who is responsible for any coordination with the Contractor. However, all correspondence to or authorization from the Board shall be made with the Member Secretary on following Address:

Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, opp. Cine planet, Near Sion Circle, Sion, (East), Mumbai – 400 022.

18.0 WARRANTY/O&MCONTRACT

18.1 All the MCAAQMV's shall be under O&M Contract from the date of successful commissioning of the MCAAQMV's. The details terms and conditions and

scope of work during O&M Contract period shall be as specified in the Scope of Work, Section - II of this document.

18.2 However, the Contractor shall warrant to the Board that the Equipment to be supplied under the Contract is new, unused, of the most recent or current models, and that they incorporate all recent improvements in design and materials unless provided otherwise in the Contract. This warranty includes all spare parts and services to keep the instruments and equipment in operating condition. In case O & M is not awarded / terminated the equipment shall remain warranted for 3 years.

The Contractor shall further warrant to the Board that the Equipment complies strictly with the Specifications and has no defect, arising from design, materials, or workmanship or from any act or omission of the Contractor that may develop under normal use of the supplied Equipment in the conditions prevailing to the final Sites.

18.3 Period of O&M Contract

This O&M Contract shall remain operative for the period specified in SCC after the successful installation & commissioning of the Air Quality Monitoring System by the Contractor.

18.4 In Case of Faulty Equipment

If any part of the Equipment breakdowns or fails due to faulty of improper design, materials, workmanship, manufacture, fabrications or instructions, or fails to meet the requirements of the Specifications, then the Contractor or his O&M partner shall promptly notify the manufacturer in writing of any claims arising under this clause.

Contractor or his O&M partner shall ensure that within the period specified in Scope of Work for O&M Contract in Section - II of the document and with all reasonable speed, the repair of replacement of the defective Equipment or improper parts thereof is carried out at the Contractor's expenses.

In the event that any part of the Equipment becomes defective due to no fault of the Contractor, such as voltage fluctuations, misuse and negligence, the Contractor will be indemnified by the Board in respect of repair thereof.

18.5 Manufacturer's Warranty

The contractor must take into account any manufacture's standard Warranty on the equipment supplied **before quoting for O&M cost for the years** for which such Warranty is applicable.

19.0 INSURANCE

The Equipment supplied under the Contract shall be fully insured

(Comprehensive) in currency acceptable as per the existing Law of India against loss or damage incidental of manufacture or acquisition, transportation, storage, shipment, delivery, installation and training involved with the Works naming the Board as the beneficiary, in the manner specified in the SCC, until issuance of taking over certificate.

20.0 INSTALLATION

20.1 All the Equipment shall be installed and brought into suitable conditions for operation by the Contractor at the Sites designated by the Board. The Contractor shall make all the necessary and proper adjustments and arrangements, including, but not restricted to, the utility supplies and connections, foundation and erection works specified in Clause 3 of S/W in order to install the Equipment in adequate conditions for operation.

All matters omitted from this Clause which may reasonably be incurred to be obviously necessary for the proper installation and operation of the Equipment shall be deemed to be included in this installation works, and the Contractor shall be held responsible for any errors or defects which the Contractor may make due to such omissions thereof.

- 20.2 Only the best installation practices are to be applied, and all the installation works must be done to the satisfaction of the Board and the Contractor shall carry out his works in a neat and proper workmanlike manner. The installation shall be planned and carried out in no way to damage installation materials and the Equipment.
- **20.3** All the installing Equipment, tools, materials, labour, logistics and all the other requirements for installation shall be provided by the Contractor.
- 20.4 Prior to the establishment of Equipment layout and installation plan, the Contractor shall verify, check and inspect the designs and specific site conditions of monitoring vans and laboratories where the Equipment are to be installed so as to make good arrangement for installation and utility assembly in consultation with the Board.

21.0 INSPECTION AND TEST

- 21.1 The Board shall have the right to inspect and the test the Equipment to confirm their conformity to the Specifications without any extra charge to the Board by the Contractor. The Contractor shall notify the Board, in a timely manner (at least 21days in advance), of the schedule of inspections and test.
- 21.2 The inspections and test shall be conducted on the premises of the Contractor and/or the Manufacturers and the Sites. If conducted on the premises of the Contractor and/or the Manufacturers, all reasonable facilities and assistance, including access to drawings and production

- data, shall be furnished to the Inspection Team for the inspections and test at no charge to the Board.
- 21.3 Should any inspected or tested Equipment fail to conform to the Specifications, the Board may reject the Equipment, and the Contractor shall either replace Equipment or make alternations necessary to meet the Specifications requirements free of cost to the Board.
- 21.4 No pre dispatch inspection is envisaged for equipment of foreign origin and contractor shall furnish factory test / inspection reports as furnished below of the manufacturer along with the dispatch documents. However, the Board reserves the right to appoint at its cost, any inspection agency (other than suggested by contractors) which will be binding on the contractor.
 - →Performance Test Certificate of all analyzer/ UPS/ 1.2 mm pre- coated GI Sheet of container, NIST traceability for gas Aluminum cylinders / Permeation tube.
 - → Certificate of Traceability
 - → Verification of System Completeness
 - → Product Certificate
- 21.5 For the equipment of Indian origin contractor should submit check list for equipment for approval of MPCB. For container, contractor should take prior approval of the drawing from MPCB. Contractor should notify date of pre-dispatch inspection to the MPCB at least 15 (fifteen) days ahead of inspection.
- 21.5 The Board's right to inspect, test and, where necessary, reject the Equipment after the Equipment's arrival in India shall in no way limited or waived by reason of the Equipment having previously been inspected, tested and passed by the Board prior to the Equipment's shipment from the country of origin.

Inspections and Tests

Manufacturer's test and inspection certificate to be provided along with the Supply Inspection and tests prior to shipment of Goods and at final acceptance are as follows:

- Inspection: The Drawing of each of the equipment is to be certified by a qualified expert as may be nominated by the Member Secretary, Maharashtra Pollution Control Board - Mumbai. The equipment shall be inspected if required at the manufacturer's place in India or its dispatch facility in India, prior to dispatch and also after successful installation at respective site by Officials / expert, nominated by the Member Secretary, Maharashtra Pollution Control Board. Such authority shall issue the inspection and clearance certificate which will be a mandatory document for release of payments of 80 %.
- (ii) The inspection of the goods shall be carried out to check whether the instruments are in conformity with the technical specifications contained in the bid document and attached with the letter of

acceptance and shall be in line with the inspection/test procedures laid down in the technical specifications and the. manufacturer's certificate. The purchaser will test the equipment at the manufacturer's place dispatch and also after completion of the installation and commissioning at the site of the installation. For site preparation, the supplier should furnish all details to the purchaser sufficiently in advance so as to get the works completed before receipt of the equipment. Complete hardware and software as specified in bid document should be supplied, installed and commissioned properly by the supplier prior to commencement of performance tests.

(ii) The acceptance test will be conducted by a committee/Officials appointed by The Member Secretary, Maharashtra Pollution Control Board, Mumbai will inspect and make recommendation on the acceptance of material.

At its option the committee co-opt any other subject matter can specialist to facilitate the inspection. The acceptance will involve troubleoperation for consecutive davs. There shall seven not additional charges for carrying out acceptance tests. No malfunction, partial or complete failure of any part of hardware or excessive heating and sub-systems attached to instruments should occur. supplier shall maintain necessary log in respect of the results of the tests establish satisfaction of the purchaser, the successful the entire completion of the test specified. An average uptake efficiency of 98% (to modify as considered appropriate for each case) for the duration of test period shall be considered as satisfactory.

(iii) In the event of the hardware and software failing to pass the acceptance test, a period not exceeding two weeks will be given to rectify the defects and clear the acceptance test, failing which the purchaser reserves the rights to get the equipment replaced by the supplier at no extra cost to the purchaser.

Manuals and Drawings

- (a) Before the goods and equipment are taken over by the Purchaser, the Supplier shall Supply, Operation and maintenance manuals together with drawings of the goods and equipment. These shall be in such detail as will enable the Purchaser to operate, maintain, adjust and repair all parts of the works as stated in the specifications.
- (b) The manuals and drawings shall be in the ruling language (English) and in such form and numbers as stated in the contract.
- (c) Unless and otherwise agreed, the goods and equipment shall not be considered to be completed for the purpose of taking over until such manuals and drawings have been supplied to the Purchaser.

For the System and Other Software the following will apply:

The Supplier shall provide complete and legal documentation of hardware and all subsystems so necessary for operation of the equipments. The supplier shall also indemnify the purchaser against any levies/penalties on account of any default in this regard.

Acceptance Certificates:

- (a) On successful completion of acceptability test, receipt of deliverables etc, and after the purchaser is satisfied with the working on the equipments, the acceptance certificate signed by the supplier and the members of committee/officials will be issued. The date on which such certificate is signed shall be deemed to be the date of successful commissioning of the systems.
- (b) The training as specified in Technical Specifications shall be conducted on the dates mutually agreed upon and within two months from the date of acceptance of Commissioning of MCAAQMV.

22.0 TRAINING

- 22.1 The Contractor shall provide the Board staff with the training as specified in Clause 5 of S/W for the Equipment & Technical Specification.
- 22.2 The Contractor shall furnish the schedule and program of the training to the Board within 30 days after the notification of award in such a manner that proper training is imparted to Board staff members.

23.0 COMPLETION

The Contractor shall complete all the Works by the date as specified in SCC.

23.1 Taking Over

Upon successful completion of delivery, installation, inspection and training of the Equipment to and at the designated Sites and O&M of the MCAAQMV for the period specified in S.C.C., the Contractor shall notify the Board in writing that all the Works under the Contract have been completed at least 30 days before expiry of O&M Contract period.

Immediately after completion of O&M Contract period as specified in S.C.C., the Board will take over the Mobile Continuous Ambient Air Quality Monitoring Vans or make alternate arrangement for their O&M.

24.0 SUBMISSION OF DOCUMENTS

The Contractor shall submit the documents specified in SCC to the Board. The Contractor shall prepare all the documents in English.

Besides the documents thereof, the Contractor shall submit the notices, reports, and other documents when deemed necessary, in accordance with the direction of the Board.

25.0 PAYMENT

25.1 Payment

The method, terms and conditions of payment to be made to the Contractor under this Contractshall be specified in SCC. The Contractor's request(s) for payment for, as appropriate, the Equipment delivered and the Works performed and fulfillment of other obligations stipulated in the Contract shall be made to the Board in writing, accompanied by documents specified in SCC.

25.2 The payment shall be made promptly by the Board but in no case not later than sixty (60) days after submission of invoice or claim by the contractor.

25.3 Currency of Payment

The currency in which payment is made to the Contractor under this Contract shall be specified in SCC.

26.0 PRICES

Prices charged by the Contractor to the Board for the Equipment delivered and the Works performed under the Contract shall not vary from the prices quoted by the Contractor in the Financial Bid.

27.0 PERFORMANCE SECURITY

27.1 Performance Security

The Contractor within thirty (30) days from the date of notification of award shall furnish a Bank Guarantee from a reputed Indian or Nationalized Commercial Bank having license to do business in India to the Board in line with the enclosed from as per Attachment 1 Section VI towards performance guarantee for an amount equal to ten (10 %) percent of the total Price under the Contract for faithful and due fulfillment by the Contractor of all obligations under the terms and conditions of the Contract. (Valid up to 1 Year from date of Successful installation and Commissioning) [Attachment -1, Section VI]. The Bank Guarantee from Indian Nationalized Bank for Operations and Maintenance Service shall furnish before signing the contract agreement by contractor for an amount equal to four (4) quarterly O & M Charges. (Valid for 5 Year O & M Service Period). [Attachment -4, Section VI]

The Contractor shall ensure that Contract Performance Security remains valid at one

year after commissioning of entire system satisfactorily.

27.2 Return of Performance Security

The performance security (guaranty) will be discharged by the Board and returned to the Contractor not later that forty-five (45) days after expiry of one year subject to date of completion of the Contractor's performance obligations under the Contract, including obligations, unless specified otherwise in SCC.

28.0 ASSIGNMENT

The Contractor shall not assign in whole or in part, its obligations to perform under this Contract, except with the Board's prior written consent.

29.0 SUBCONTRACTORS

29.1 The Contractor shall notify the Board in writing of all the Manufacturers awarded under this Contract and any other subcontractors involved with performance of the Works if not already specified in the Bid. Such notification, in the original Bid or later, shall not relieve the Contractor from any liability or obligation under the Contract.

30.0 DELAYS IN THE CONTRACTOR'S PERFORMANCE

30.1 Delays in the Contractor's Performance

Delivery of the Equipment and performance of the Works shall be made by the Contractor in accordance with the time schedule specified in SCC.

30.2 Notification of Delay

If at any time during performance of the Contract, the Contractor and/or the Manufacturers should encounter conditions impending timely delivery of the Equipment and performance of the Works, the Contractor shall promptly notify the Board in writing of the fact of the delay, its likely duration and its cause(s). As soon as practicable after receipt of the Contractor's notice, the Board shall evaluate the situation and may at its discretion extend the Contractor's time for performance, with or without liquidated damages, in which case the extension shall be ratified by the Board by amendment of the Contract.

30.3 Liability of Liquidated Damages

Except as provided under Clause 34 of GCC, a delay by the Contractor in the performance of its delivery obligations shall render the Contractor liable to the imposition of liquidated damages pursuant to Clause 31 hereunder, unless an extension of time is agreed upon pursuant to Sub-

clause 30.2 here above without the application of liquidated damages.

31.0 LIQUIDATED DAMAGES

If the Contractor fails to perform the Works within the period specified in Clause 11 of SCC, the Board shall, without prejudice to its other remedies under the Contract, deduct from the Contract Price, as liquidated damages, a sum equivalent to the percentage specified in SCC. Once the maximum is reached, the Board may consider termination of the Contract pursuant to Clause 35 of GCC.

32.0 SUSPENSION OF WORK

The Contractor shall not suspend the whole or any part of the Works without notice to the Board in writing. The Contractor thereupon shall do all possible endeavors to reduce any expenses or costs resulting from the suspension. Such suspension shall not nullify the Contract.

33.0 TERMINATION FOR DEFAULT

33.1 Termination for Default

The Board, without prejudice to any other remedy for breach of Contract, by written notice of default sent to the Contractor, may terminate this Contract in whole or in part:

 If the Contractor fails to perform any or all of the Works within the period specified in Clause 11 of SCC, or extension thereof granted by the Board pursuant to Clause 32 of GCC

or

2) If the Contractor fails to perform any other obligations under the Contract.

33.2 Liability for Excess Cost for Unperformed Work

In the event the Board terminates the Contract in whole or in part pursuant to Sub-clause 33.1 here above the Board may procure at the risk and cost of the contractor, upon such terms and in such manner as it deems appropriate, the equipment / works similar to those undelivered / unperformed and the Contractor shall be liable to the Board for any excess costs for such similar equipment / works. However, the Contractor shall continue performance of the Contract to the extent not terminated.

34.0 FORCE MAJEURE

34.1 Notwithstanding the provisions of Clauses 32, 33 and 35 in GCC, the Contractor shall not liable for forfeiture of its performance security, liquidated damages, or termination for default if and to the extent that its delay in performance or other failure to perform its obligations under the Contract is the result of an event of Force Majeure.

- 34.2 For the purposes of this Clause, "Force Majeure" means an event beyond the control of the Contractor and not involving the Contractor's fault or negligence and not foreseeable. Such events may include, but are not restricted to, acts of the Board in its sovereign capacity, wars or revolutions, fires, floods, epidemics, quarantine restrictions, and freight embargoes.
- 34.3 If a Force Majeure situation arises, the Contractor shall promptly notify the Board in writing of such condition and the cause thereof. Unless otherwise directed by the Board in writing, the Contractor shall continue to perform its obligations under the Contract as far as is reasonably practical, and shall seek all reasonable alternative means for performance not prevented by the Force Majeure event.

35.0 TERMINATION FOR INSOLVENCY

The Board at any time terminates the Contract by giving written notice to the Contractor if the Contractor becomes bankrupt or otherwise insolvent. In this event, termination will be without compensation to the Contractor, provided that such, termination will not prejudice or affect any right of action or remedy which has accrued or will accrue thereafter to the Board.

36.0 RESOLUTION OF DISPUTES

36.1 Settlement of Disputes

Any dispute(s) or difference(s) arising out of or in connection with the Contract shall, to the extent possible in the first instance be resolved amicably between the Contractor and the Owner's.

If, after thirty (30) days, the parties have failed to resolve their dispute or difference by such mutual consultation, then either the Purchaser or the Contractor may give notice to the other party of its intention to commence arbitration, as hereinafter provided, as to the matter in dispute, and no arbitration in respect of this matter may be commenced unless such notice is given.

Any dispute or difference in respect of which a notice of intention to commence arbitration has been given in accordance with this Clause shall be finally settled by arbitration. Arbitration may be commenced prior to or after delivery of the Goods under the Contract.

In the case of dispute or difference arising between the Purchaser and a Domestic Contractor relating to any matter arising out of or connected with this agreement, such disputes or difference shall be settled in accordance with the Arbitration and Conciliation Act, 1996. The arbitral tribunal shall consist of (3) three arbitrators one each to be appointed by the Purchaser and the Contractor. The third arbitrator shall be chosen by the 2 (two) Arbitrators so appointed by the parties and shall act as

Presiding arbitrator. In case of failure of the two arbitrator appointed by the parties to reach upon a consensus within a period of 30 days from the appointment of the arbitrator appointed subsequently, the Presiding Arbitrator shall be appointed by the President of the Institution of Engineers (India).

In case of a dispute with a Foreign Contractor, the dispute shall be settled in accordance with provision of UNCITRL (United Nations Commission on International Trade Law) Arbitration Rules. The Arbitral Tribunal shall consist of three Arbitrators one each to be appointed by the Purchaser and the Contractor. The third Arbitrator shall be chosen by the two Arbitrators so appointed by the Parties, and shall act as presiding arbitrator. In case failure of two arbitrators appointed by the parties to reach upon a consensus within a period of 30 days from the appointment of the arbitrator appointed subsequently, the Presiding Arbitrator shall be appointed by the President of the Institution of Engineers (India).

If one of the parties fails to appoint its arbitrator in pursuance of SubClause (a) and (b) above, within thirty days after receipt of the notice of the appointment of its arbitrator by the other party, then the Presiding Arbitrator shall be nominated by President of the Institution of Engineers (India), both in case of the foreign contractor as well as Indian Contractor, shall appoint the arbitrator. A certified copy of the order of the President of the Institution of Engineers (India), making such an appointment shall be furnished to each of the parties.

Arbitration proceedings shall be held at Mumbai, Maharashtra, India, and the language of the arbitration proceedings and that of documents and communications between the parties shall be English. The decision of the arbitrators final binding upon both parties. The shall be and cost and expenses of Arbitration proceedings will be paid as determined by the arbitral tribunal. However, the expenses incurred by each party in connection with the preparation, presentation etc. of its proceedings as also the fees and expenses paid to the arbitrator appointed by such party or on its behalf shall be borne by each party itself. Where the value of the contract is Rs. 10 million and below, the disputes or differences arising shall be referred to the Sole Arbitrator. The sole Arbitrator should be appointed by agreement between the parties; failing such agreement, by the appointing authority namely the President of the Institution of Engineers (India).

37.0 TAXES AND DUTIES

- a) Presently, Concessional Customs Duty (CCD) shall be applicable on the equipment being imported by Maharashtra Pollution Control Board. Necessary exemption certificate shall be issued by MPCB and applicable Custom Duty after claiming concession, if any such Custom Duty shall be paid/reimbursed by MPCB at actuals.
- b) MPCB is also exempted from paying Excise Duty. Necessary

- exemption certificate shall be issued by the MPCB.
- c) Local taxes or any other taxes applicable will be paid/reimbursed to the supplier by MPCB at actual against documentary evidence.
- d) Taxes on incidental services like Installation, Commissioning and training and O&M service etc. shall be payable extra at actuals by MPCB.

38.0 INJURY AND DAMAGE

38.1 Injury or Death of Persons

The Contractor shall be liable for and shall indemnify the Board against any liability, loss claim or proceedings whatsoever arising under any statue or law in respect of personal injury or death or any disability caused by the carrying out of the Works unless due to any act or neglect of the Board, or of any person for whom the Board is not responsible.

Without prejudice to the Contractor's liability to indemnify the Board, the Contractor shall maintain and cause any manufacturers and subcontractors to maintain such insurance as necessary to cover the liability of the Contractor or, as the case may be, of such Manufacturers and subcontractors, in respect of personal injuries of deaths arising out of or in the course of or caused by the carrying out of the Works.

38.2 Damage to Property

The Contractor shall liable for and indemnify the Board against and insure any Manufacturers and subcontractors to insure against any expense, liability, loss claim or proceedings in respect of any damage whatsoever to any real or personal property for any one occurrence in so far as such damage arises out of or in the course of or by reason of the carrying out of the Works and is due to any negligence, omission or default of the Contractor or any person for whom the Contractor is responsible or any Manufacturers and subcontractors or person for whom the Manufacturers and subcontractors are responsible.

39.0 ROYALTY AND PATENTS

39.1 The Contractor shall pay all royalties and licenses fees for the use of any patented item, whether it may be an invention, method, arrangement,

article, process or appliance used in connection with the performance of the Contract. The Contractor shall indemnify and save harmless the Board against any and all costs, damages and expenses of any nature or kind whatsoever which may arise out of or result from a claim by any person, firm or corporation that the manufacture, purchase, use of sale

of any of the inventions, methods, arrangements, articles processes or appliances used in connection with the performance of this Contract infringes any patent of such

other rights. The Contractor shall, at the request of the Board, defend the Board against any suit brought to enforce any such claim at the Contractors expense.

39.2 In case any such patented item used on or in conjunction with the Works is in suit held to constitute and infringement of its use enjoined, the Contractor shall either secure for the Board the right to continue using the said item by suspension of the enjoinment, by procuring for the Board a license or otherwise, or will replace such items with a non-infringing item or modify it so that it becomes non-infringing or with the Board's approval remove the said enjoined item and refund to the Board the sums paid thereof.

40.0 EFFECTIVENESS

This Contract shall come into force and effect on the date of the Letter of Award and shall be in force until the Works have been completed and all the payments have been made to the Contractor, including the payments for O & M contract period.

41.0 LAWS AND REGULATIONS


The formation, validity and performance of this Contract shall be governed as to all matters by and under the laws and regulations of India and courts in Mumbai, Maharashtra shall have exclusive jurisdiction in all matters arising under this Contract.

The Contractor shall respect and abide by all laws and regulations of India and shall make its best effort to ensure that the personnel of the Contractor and their dependents, while staying in India, shall respect and abide by all laws and regulations of India. The Contractor shall protect, absolve and indemnify the Board and their representatives from any claim, loss or damage arising from any non-compliance alleged or proved, without claiming them for payment.

42 NOTICES

Any notice given by one party to the other pursuant to this Contract shall be sent to the other party in writing or by cable, telex, facsimile and confirmed in writing to the other party's address specified in SCC.

A notice shall be effective when delivered or on the notice's effective date, whichever is later.

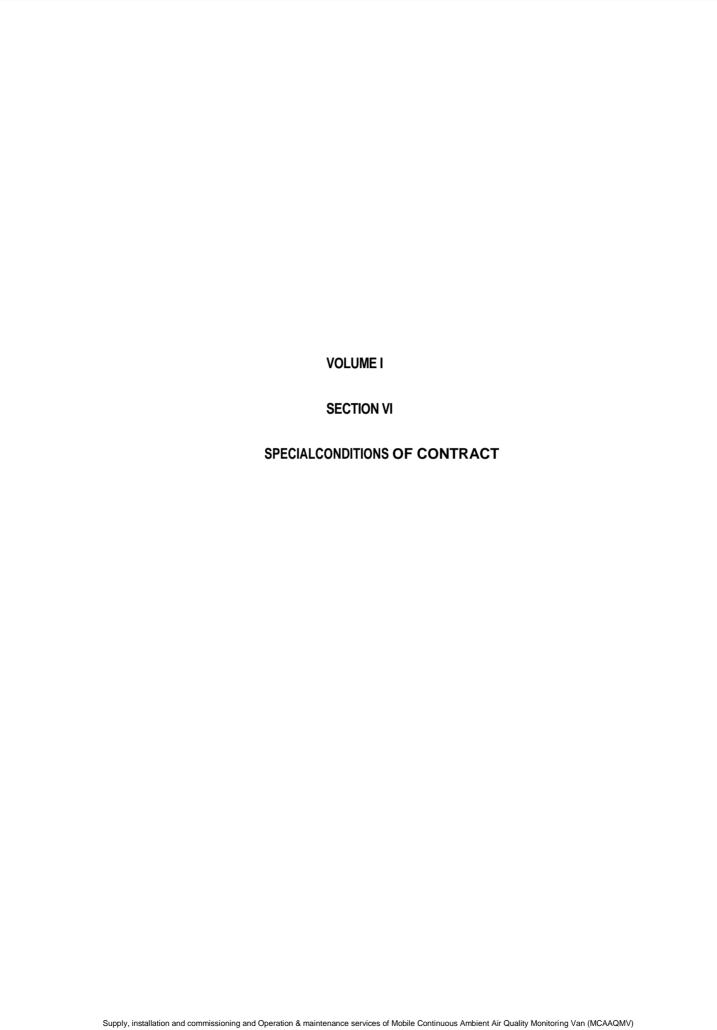

SECTION VI

Sr. No	b. SPECIAL CONDITIONS OF CONTRACT CONTENTS	Page no.	
1.	Climate Condition	113	
2.	Consumables and Spare Parts	113	
3.	Name Plate	113	
4.	Marking	114	
5.	Shipment	114	
6.	Works Schedule	116	
7.	Warranty / O&M Contract	117	
8.	Insurance	117	
9.	Installation	117	
10.	Inspection and Test	117	
11.	Completion	118	
12.	Submission of Documents	119	
13.	Payment	120 to 12	1
14.	Prices	122	
15.	Performance Security	122	
16.	Liquidated Damages	122	
17.	Notices	122	
Attach	ment 1 : Performance Security Form	131 to 132 A	Attachment 2 :
Form	for Contract Agreement	to 136	
	nment 3 : Proforma of Certificate for issue by the Mi	PCB After Successful	Commissioning
Atta	chment 4 Proforma for Bank Guarantee by O&M F	Partner 138 to 140	

SPECIAL CONDITIONS OF CONTRACT

The following Special Conditions of Contract shall supplement the General Conditions of Contract. Whenever there is a conflict the provisions herein shall prevail over those in the General Conditions of Contract the corresponding clause number of the GCC is indicated in parentheses, if applicable.

1.0 CLIMATE CONDITION

Precaution and protection against the specific climate conditions in India such as heavy rain, high temperature, high humidity, gales, excessive sunshine, flooding or any other climate conditions which could cause damage upon the Equipment or otherwise interfere with the execution of the works shall be taken. The Equipment to be supplied shall be tropicalized.

2.0 CONSUMABLES AND SPARE PARTS

2.1 Supply of Consumables and Spare Parts

The Contractor shall provide the consumables and spare parts as per requirement of Operation & maintenance of Air Quality Monitoring Analysers System.

2.2 After Sales Services

The Contractor shall guarantee the availability of all consumables, spare parts, maintenance and repair work for each Equipment at cost basis for at least five (5) years after the O&M period specified in Clause 7 of SCC, unless otherwise specified in the Specifications.

Bidder should submit certificates from the manufacturers in support of available service centers and availability of spares parts and consumable in India as per Attachment no. 3A of Section III.

3.0 NAME PLATE (GCC CLAUSE 12)

The Contractor shall affix the name plate with the following description in English on all the Equipment:

- 1) Name of the station
- 2) Name of the Equipment
- 3) Manufacturing date
- 4) Production serial number
- 5) Equipment model number

- 6) Name of manufacturer
- 7) Ratings of the Equipment
- 8) Logo of MPCB.

4.0 MARKING (GCC SUB-CLAUSE 13.2)

The Contractor shall mark the following information in the sequence described below and, in a frame, commensurate with the size of packing and/or the Equipment.

- 1) Consignee: (Maharashtra Pollution Control Board & Address), India
- 2) Name of the Works: Supply and O&M of Mobile Continuous Ambient Air Quality Monitoring Vans (MCAAQMV) for MPCB for the following stations:

List of the City / Locations where 15 nos. of MCAAQMV shall be delivered:

- 1) Locations mentioned at Invitation for Bids (IFB).
- 2) Name of the Project: Supply and O&M of Mobile Continuous Ambient Air Quality Monitoring Vans (MCAAQMV):
- Contract number:
- Contractors name:
- Port or airport of discharge:
- Country of origin:
- Item, and if applicable, package number in sequence, and quantity per package and/or Equipment:
- Description of Equipment:
- Net and gross weight and cubic measurement:
- Shipper's name and/or marks:
- Caution marks, if applicable:
- 3) Other markings as required by the Board:

5.0 SHIPMENT (GCC CLAUSE 14)

The Contractor shall be responsible for the delivery of the Equipment to each Site designated by the Board and for the coverage of shipping charges, freight, insurance premiums up to handling over the Equipment at Sites, inland transportation and temporary storage.

5.1 Notification and Submission of Documents

Upon shipment, the Contractor shall notify the Board and the Insurance Company by cable of the following details of the shipment.

- 1) Contract number
- 2) Description and quantity of the Equipment
- 3) Name of vessel and air cargo
- 4) Number and date of bill of lading and airway bill
- 5) Date of shipment, port of discharge, expected date of departure and expected date of arrival
- 6) Invoice amount of shipment
- 7) Name of a claim settling agency in India.
- **5.2** The Contractor shall mail the following documents to the Board, with a copy to the Insurance Company.

(1) Equipment of Foreign Origin:

- i) Four (4) Copies of the contractor's invoice showing the Equipment's description, quantity, unit price and total amount
- ii) Original and Four (4) copies of the negotiable, clean, on-board bill of lading marked freight prepaid and four copies of non-negotiable bill of lading;
- iii) Four copies of the packing list identifying contents of each package
- iv) Insurance certificate
- v) Manufacturer and Suppliers warranty certificate vi) Factory

test and inspection certificate

vii) Certificate of country-of origin

The above documents shall be received by the Board at least one week before arrival of the Equipment at the port or place of arrival and. If not received, the Contractor will be responsible for any consequent expenses.

Partial shipment and transhipment is allowed but within the stipulated time period:

(2) Equipment to be supplied from within India:

Upon delivery of the Equipment to the transporters, the Supplier shall notify the Board and mail the following documents to the Board.

- Four copies of the Supplier's invoice showing the Equipment's description, quantity, unit price and total amount
- ii) Acknowledgement of receipts of goods from the consignee i.e. receipted delivery note, railway receipt (RR), or truck receipt (LR)
- iii) Supplier's and/or Manufacturer's warranty certificate
- iv) Factory test & inspection certificate and Material Dispatch Clearance Certificate (MDCC) issued by the Board.
- v) Insurance certificate
- vi) Certificate of country of origin

The above documents shall be received by the Board before arrival of the Equipment and, if not received, the Supplier shall be responsible for any consequent expenses.

6.0 WORKS SCHEDULE (GCC CLAUSE 16)

6.1 Equipment to be supplied from Foreign Country:

Delivery Period for all the packages shall be **90 days from the date of the opening of Letter of Credit (L/C).** It relates to completion of delivery on CIF (designated Sea Port / Air Port) basis for equipment of foreign origin. Further transportation to the site where the MCAAQMV's is to be installed and commissioned shall be completed by the contractor **within Sixty (60) days** from the date of arrival of equipment at port of de- embarkment.

6.2 Equipment to be supplier from India:

All the equipment shall be received at Continuous Ambient Air Quality Monitoring Station Sites within 90 days from the date of notification of award and are to be installed and commissioned within sixty (60) days from date of receipt at site.

6.3 Commissioning and others incidental services:

All the equipment of the awarded package shall be commissioned within **120** days after the date of opening of Letter of Credit (L/C) including all the incidental services i.e. training etc.

6.4 O & M Contract

The contractor shall carry out Operation & Maintenance of Air Monitoring System for a period of five (5) years from the date of commissioning of the station, which can be extended up to extended

(3) Years at all mutually agreed rates and terms & conditions.

7.0 WARRANTY/O & M CONTRACT (GCC CLAUSE 18)

7.1 Period of O&M Contract

The Continuous Ambient Air Quality Monitoring System shall be under Operation & Maintenance Contract from the date of commissioning of the station and maintenance of all the equipment including Supply of all material shall be the responsibility of the Contractor during the validity of Operation & Maintenance Contract. The Contractor shall, in addition, comply with the performance guarantees if specified under the Contract. If, for reasons attributable to the Contractor, these guarantees are not attained in whole or in part, the Contractor shall make such changes, modifications, and/or additions to the Equipment or any part thereof as may be necessary in order to attain the contractual guarantees specified in the Contract at its own costs and expenses and to carry out further performance test.

8.0 INSURANCE (GCC CLAUSE 19)

- A) The insurance (Comprehensive) shall be in an amount of equal to One Hundred Ten (110) percent of the value of the Equipment up to handing over of the Equipment to the Board on "All Ricks" basis, including war risks and strikes, naming the Board as the beneficiary.
- B) The Contractor shall take the comprehensive all risk insurance cover for the complete station during O&M period including statutory insurance of Contractor's personnel. The value shall be 110% of the total value of the Mobile Continuous Ambient Air Quality Monitoring Vans depreciated annually as per standard norms. The same shall be reimbursed by the Board against documentary proof.

9.0 INSTALLATION (GCC CLAUSE 20)

Bidder shall depute Engineer / supervisor for on-site assembly, installation, commissioning and start-up of the supplied equipment. Bidder shall also furnish tools required for assembly, commissioning and maintenance of equipment during O&M period.

10.0 INSPECTION AND TEST (GCC CLAUSE 21)

10.1 Unpacking Inspection

Unpacking inspection shall be performed by the Contractor to inspect whether all the items and quantity of the Equipment have been delivered in conformity with the Equipment and packing list without any damage during the shipment.

The Contractor shall submit the unpacking inspection report to the Board.

10.2 Site Inspection

The Contractor shall carry out site inspection of the Equipment at each Site at the completion of installation works to confirm that the installation works and the function of the Equipment is satisfactory for the requirements specified in S/W and the Specifications.

The Contractor shall carry out the functional test to ensure that the consumables and spare parts are good for the operation, maintenance and replacement in future.

As a result of site inspection, the Equipment regarded as unsatisfactory or unacceptable by the Board shall be promptly remedied by the contractor. The Contractor shall submit the site inspection report to the Board.

10.3 Performance Test

The Contractor shall carry out the performance test to inspect and witness the function of each of the equipment supplied under the awarded package at site.

Performance test shall be carried out in accordance with Sub-clause 4 of S/W for all the Equipment supplied.

In case the Equipment for performance test requires the supplemental and/or supporting Equipment, the Contractor shall carry out the performance test including such Equipment.

Performance test will be considered to be complete only after successful completion of performance test of each equipment pertaining to respective packages.

In case of results of such performance test found to be unsatisfactory by the Board same shall be promptly reminded by the Contractor.

The Contractor shall prepare the performance test procedures for approval by the Board at least thirty (30) days prior to the testing schedules.

The Contractor submits the performance test report to the Board.

11.0 COMPLETION (GCC CLAUSE 23)

The Contractor shall complete all the Works up to installation and commissioning of MCAAQMV's within 180 days after the date of opening of Letter of Credit (LC).

12.0 SUBMISSION OF DOCUMENTS (GCC CLAUSE 24)

12.1 Work Program

Within thirty (15) days from the notification of award of the Contract, the Contractor shall submit the detailed Works program and schedule to the Board indicating the following items:

- a. Equipment Supply program and Equipment layout plan (if applicable)
- b. Design drawings and utility list, if required
- c. Subcontractor list for installation work of the Equipment if not already specified in the Techno-commercial Bid
- d. Program for factory, pre-shipment, unpacking and site inspections and performance test
- e. Installation program including personnel organization chart of the Contractor.

The Contractor shall be responsible for any discrepancies, errors or omissions or delay in delivery and submission of the work program, and any expenses resulting there from shall be borne by the Contractor.

12.2 Other Documents

The Contractor shall submit the following documents within forty five (45) days after the notification of ward.

Item	Number of Documents to be		
	sent to MPCB		
Catalogues, product data and test reports	4		
Installation manuals	4		

Manufacture's specifications	4
Training program	4

Besides the documents here above, the Contractor shall submit the following documents at the designated time for submissions as follows:

Item	Number of Document	Time of Submission			
	Board				
Inspection report	2	At the time of completion of factory, pre-shipment unpacking and site inspections (if applicable)			
Training manual	10	At the time of commencement of installation of Equipment			
Operation and	10	At the time of commencement of			
Maintenance manual		installation of Equipment			
Training program	1	By the time of completion of			
		installation of Equipment			
Report of performance	1	At the time of completion of			
test		performance test			
Video CD (Optional)	1	By the time of commencement of training			
List of Equipment supplied	2	At the time of completion of the Work			

Besides the documents here above, the Contractor shall submit the notices, reports, and other documents when deemed necessary, in accordance with the direction of the Board.

13.0 PAYMENT (GCC CLAUSE 25)

13.1 Method of Payment

The payment shall be made in the currency specified in the contract by means of an irrevocable Letter of Credit (LC) for equipment against dispatch. Other payment shall be made through Cheque /Bank transfer only.

13.2 Terms and Conditions of Payment

Bids with terms and conditions of payment other than that specified below shall be rejected.

- (a) Payment for goods and services (excluding O&M charges) supplied from abroad:
- i) On shipment: Eighty (80) percent of the contract price of the Supply, installation and commissioning and Operation & maintenance services of Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV)

Page 120 of 253

Goods shipped shall be paid through irrevocable Letter of Credit opened in favour of the supplier in a bank in his country and upon submission of the documents specified in sub-clause 5.2 (1) of SCC including: (i) Packing list and (ii) Supplier's certificate that the amounts shown in the invoice are correct in terms of the contract and that all the terms and conditions of the contract have been complied with and

- ii) On Final Acceptance: Balance Twenty (20) percent of contract price of the equipment including 100% of the local costs, incidental cost, cost of training after satisfactory completion of installation &commissioning including Training (to be certified by the Board) of all the Equipment of the package at specified site(s) and submission of acceptance certificate as per Attachment 3 of SCC.
- iii) 100% Payment of local currency portion including agency commission shall be paid after satisfactory completion of installation & commissioning including Training (to be certified by the Board) of all the Equipment that specified site(s).
- (b) Payment of goods and services (excluding O&M charges) supplied from India.
- On Delivery: Eighty (80) % of the contract price shall be paid (Through LC) on receipt of Goods and upon submission of the documents specified in Clause 5.2 (2) of SCC: and
- ii) On Final Acceptance: Balance Twenty (20) percent of contract price of the equipment including 100% of the local costs, incidental cost, costs of training after satisfactory completion of installation & commissioning including Training (to be certified by the Board) of all the Equipment of the particular package at specified site and submission of acceptance certificate as per Attachment 3 of SCC.
- (c) Payment of Operation and Maintenance charges:

O&M cost of each year shall be paid after end of every quarter in equal installments based on submission of required air quality report as per annexure X1 to X5 along with data obtained from calibration documentation. Any penalties applicable if any as referred in Scope of Work for O&M Contract and as per notification of award of contract shall be deducted from the quarterly payment.

- (d) i) Where payments are to be effected through Letter of Credit (LC), the same shall be subject to the latest Uniform Customs and Practice for documentary credit, of the International Chamber of Commerce.
 - ii) The LC will be confirmed at Supplier's cost if requested specifically by the supplier;
 - iii) If LC is required to be extended/ reinstated for reasons not attributable to the Purchaser, the charges thereof shall be to the suppliers account.

Any expenditure for the operation of LC out - side India shall be iv) borne by the beneficiary.

14.0 PRICES (GCC CLAUSE 26)

The prices quoted shall be firm throughout the tenure of the Contract. Any increased cost incidental to the performance of the Works due to any economic dislocation either in the origin country or India or to any other causes such as currency restriction, price hike of the Equipment, wage hike for labour or revaluation of the currency can not be claimed by the Contractor to the Board.

15.0 PERFORMANCE SECURITY (GCC CLAUSE 27)

15.1 Performance Security

The amount of performance security as a percentage of the Contract Price shall be ten (10 %) percent.

16.0 LIQUIDATED DAMAGES (GCC CLAUSE 31)

16.1 Rate

The Contractor shall pay to the Board as liquidated damages a sum equivalent to half (0.5) percent of the contract price of each station for per week of delay in commissioning of each station after scheduled date of completion.

16.2 Maximum Deduction

The total liquidated damages on account of delay in supplies payable to the Board shall not in any case exceed five (5) percent of the Contract price of Supply portion only (Excluding O&M charges).

16.3 In addition to above Liquidated damages for delay, the Contractor is liable to pay penalty on account of failure of systems during O&M period as elaborated in Section - II (Scope of work) of this document.

17.0 NOTICES (GCC CLAUSE 42)

Any notice, request or consent shall be deemed to have been given or made when delivered in person to an authorized representative of the party to whom the communication is addressed or when sent by registered mail telex, telegram, facsimile to such party at the following address:

The Member Secretary,

Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, Cine Planet, Near Sion Circle, Sion (East), Mumbai – 400 022

Attachment 1

Form of Bank Guarantee for Performance Security For SUPPLY UNDER BUY-BACK, Installations, Commissioning and Testing of MCAAQMV.

(to be stamped in accordance with Stamp Act, if any, of the Country of the issuing Bank) Bank Guarantee No. -----Date: Ref. No.: To. The Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, Cine Planet, Near Sion Circle, Sion (East), Mumbai - 400 022. Dear Sir. THIS AGREEMENT is made on the -----days of----- 2016 -----Between [Name of the Bank] of -----[address of the (hereinafter called "the Guarantor") of the one part and Maharashtra Pollution Control Mumbai (hereinafter called "the Board") of Board, the other part. **WHEREAS** (1) this agreement is supplemental to a contract number -----(insert Contract Number) (hereinafter called "the Contract") made between [name of Contractor] of ----- [address of Contractor] (hereinafter called "the Contractor) of the one part and the Board of the other part whereby the Contractor agreed and undertook to execute the works of Supply and O&M of Continuous Ambient Air Quality Monitoring Station (MCAAQMV) for MPCB at against the Contract for the sum of ---------- [amount in Contract Currency] being the Contract Price; and

(2) the Guarantor has agreed to guarantee the due performance of the

Contract in the manner hereinafter appearing.

NOW, THEREFORE, the Guarantor hereby agrees with the Board as follows; (a) If the Contractor (unless relieved from the performance by any clause of the Contract or by statute or by the decision of a tribunal of competent jurisdiction) shall in any respect fail to execute the Contract or commit any breach of his obligations there under then the Guarantor will indemnify and pay the Board the aggregate sum of -----[amount of Guarantee shall be ten (10)% (Percent) of the said value of the Contract]----- [in words], such sum being payable in the types and amount of currencies in which the Contract Price is payable, provided that the Board or his Authorized Representative has notified the Guarantor to that effect and has made a claim against the Guarantor before the expiry of O&M period. (b) The guarantor shall not be discharged or released from his guarantee by arrangement between the Contractor and the Board, with or without the consent of the Guarantor, or by any alteration in the obligations undertaken by the Contractor, or by any forbearance on the part of the Contractor, whether as to payment, time, performance, or otherwise, any notice to the Guarantor of any such arrangement, alteration, or forbearance is hereby expressly waived.

This guarantee shall be valid for one year from date of successful installation and commissions of entire system as specified in the Contract.

Given under our hand on the date first mentioned above.

(Witness)

	SIGNED BY
	for and on behalf of the
	Guarantor
	(Seal of Guarantor)
in the presence of	

Attachment 2

FORM FOR CONTRACT AGREEMENT FOR SUPPLYAND OPERATION & MAINTENANCE OF MOBILE CONTINUOUS AMBIENT AIR QUALITY MONITORING VANS (MCAAQMV)

This operation and Maintenance Agreement ("Agreement") is made on thisday of by and between:
Maharashtra Pollution Control Board, India which term shall include permitted assigns and successors (Hereinafter called as "The Board" or "the Owner").
And
M/sa company incorporateda tompany incorporateda
which term shall include permitted assigns and successors (hereinafter called as "Contractor" or "the Contractor")
RECITALS
Whereas the Owner had invited Bids under reference for SUPPLYand Operation & Maintenance continuous ambient Air quality monitoring Station located at:
and M/s had submitted their bid against the aforesaid invitation to bid and Owner has accepted the bid of M/s and has decided to entrust the job of Supply and Operation & Maintenance (O&M) of the one Air Monitoring Station located at to the Contractor vide Letter of Award ref dated at a total Contract Price for complete scope of work of (Contract Price in Words and Figures) (Hereinafter "the Contract Price").
Whereas the Contractor has accepted the Letter of Award issued by the Owner in writing vide its letter no dated and has furnished Contract Performance Security for an amount of Rs [Rupeesonly] and which is initially valid up to and Owner has accepted the said Contract Performance Security.
Whereas, Contractor is having expertise in the business inter alia, of Supply and operation & maintenance of Continuous Ambient Air Quality Monitoring System and the owner has engaged the Contractor to Supply and perform operation and maintenance of
said Air monitoring System upon the terms & conditions set forth in this Agreement and the Letter of Award referred above issued by the Owner including all the documents referred in the above Letter of Award.

NOW THIS AGREEMENT WITNESSETH AS FOLLOWS:

- In this Agreement words and expressions shall have the same meanings
 as are respectively assigned to them in the Conditions of Contract referred to.
- 2. The following documents shall be deemed to form and be read and construed as part of this Agreement, viz.:
 - i) Scope of Works;
 - ii) Financial Bid;
 - iii) Technical Specifications;
 - iv) General Conditions of Contract;
 - v) Special Conditions of Contract; and
 - vi) The Board's Notification of Award.

This Contract sets forth the entire contract and agreement between the parties pertaining to the SUPPLY of the Goods described herein and Operation & Maintenance of the Air Monitoring Vans and supersedes any and all earlier verbal or written agreements pertaining to the SUPPLY of the Goods.

This Contract shall prevail over all other Contract documents. In the event of any discrepancy or inconsistency within the Contract documents, then the documents shall prevail in the order listed above.

- In consideration of the payments to be made by the Board to the Contractor as hereinafter mentioned, the Contractor hereby covenants with the Board to perform the Works and to remedy defects therein conformity in all respects with the provisions of the Contract.
- 4. The Board hereby covenants to pay the Contractor in consideration of the performance of the Works and the remedying of defects therein the Contract Price or such other sum as may become payable under the provisions of the Contract at the times and in the manner prescribed by the Contract.
- 5. Any notice under the Contract shall be in the form of letter, telex, cable or facsimile. Notices to either party shall be given at such address or addresses as such party shall specify from time to time by written notice to the other. In the absence of such notice to the contrary, notice to the Board shall be properly addressed to:

The Member Secretary, Maharashtra Pollution Control Board, Kalpataru Point, 3rd Floor, Cine Planet, Near Sion Circle, Sion (East), Mumbai – 400 022.

	And	notice	to	the	Contractor	shall	be	properly	addre	essed	to:	
	[Cont	ractor's	addı	ress a	and electroni	c transr	nissio	on address	s]			
A notice shall be effective when delivered or on the notice's effective date, whichever is later.												
					parties here ective laws			d year firs	st abo	ve wri	tten.	
							S	•	of			Authorized
								Signat	ture of	Contra	ctor	
Signe	ed, Se	aled and	d De	livere	d by the saic	I		-				
(For	the Bo	ard) in t	he p	resen	ice of							
Signe	ed, Se	aled an	d De	elivere	ed by the sai	d						
(For	the Co	ontracto	or) in	the p	presence of							

Attachment 3

PROFORMA OF CERTIFICATE FOR ISSUE BY THE MPCB AFTER SUCCESSFUL COMMISSIONING OF EQUIPMENT

No.:	Date:	
M/s		
Sub:	: Certificate of Commissioning of equipment.	
1.	This is to certify that the equipment as detailed below has / have been received in good condition along with all the standard and special accessorie (subject to remarks in Para No.2) and a set of spares in accordance with the Contract / specifications. The same have been installed and commissioned.	
	a) Contract No	
	(for import contract) g) Name of the vessel/transporter	
2.	j) Date of commissioning and performance test	
SI. No	1	
3.	The proving/performance test has been done to out entire satisfaction and personnel have been trained to operate the equipment.	
BOA	RD CONTRACTOR	

Supply, installation and commissioning and Operation & maintenance services of Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV) Page 128 of 253

He has adhered to the time schedule specified in the contract in

The contractor has fulfilled his contractual obligation satisfactorily.

Explanatory notes for filling up the certificates:

4.

a)

dispatching the documents drawing pursuant to Technical Specifications.

- b) He has supervised the commissioning of the item in time i.e. within the period specified in the contract form the date of intimation by the Purchaser in respect of the installation of the plant.
- c) Training of personnel has been done by the contractor specified in the contract.
- d) in the event of documents/drawings having not been contractor or installation and commissioning of the plant have been delayed on act of the contractor, the extent of delay should always be mentioned.

OR

The contractor has failed to fulfill h	iis contractual	obligations	with regard	to the following
i.e. instruction or training etc.				

- a)
- b)
- c)
- d)
- 5. The amount of recovery, on account of non-SUPPLY of accessories and spares is given under Para No. 2.
- 6. The amount of recovery on account of failure of the contractor to meet his contractual obligations is as indicated in endorsement of the letter.

Signature							
Name							
Designation with stamp							

Member Secretary
State Pollution Control Board

Attachment 4

PROFORMA FOR BANK GUARANTEE TOBEFURNISHEDFORO&MCONTRACT (TO BE STAMPED IN ACCORDANCE WITH STAMP ACT, IF ANY, OF THE COUNTRY OF THE ISSUING BANK)

Bank Guarantee No

						ſ	Date			•••••	
expre		n shall unl	ess repu	gment t	to the con	text or m	eaning having	thereof g	as "Emp include its awarde	s succe ed	ssors, to
ith	its	Head	Office	at(hei		referre	ed to	as.			
Quali	ity Mo	nitoring M	lobile Van	(MCAA	and Oper AQMV),vio	ration &M de Contra	aintena ct No	ance of	Continuou	s Ambie	
whic	h awa	rd is on th	e strengtl	h of Fo	rm of Cert	tificate by	the 08	&M Part	ulting in a	a for Ca	rrying
M/s (here .(O& uneq a calle Perfo to the	(hereinafter referred to as "Undertaking")given by M/s										
(here conte do he to the time or pr Any notw Emplany any that that the total that the total total that the total t	ein-afte ext or ereby e exte up to otest such ithstal other a	er referre meaning guarante nt of (Spe and/or wi demand nding any and O&M Authority. previou aarantee l	d to as the thereof, is and undecify current ithout any made by difference. The Barrs corrections	e "Bar nclude dertake ency an refere the Er ce betw or any o ak unde	nk", which its succe to pay to d amount without ences to ' mployer of veen the li dispute per ertakes no	th expresessors, and the Empt tin words on the Basending beat to revolute.	sion s dministration oloyer of and fig emur, artner" ank sha and C and C afore ar ke this Employ	hall, ur rators, e on dema gures) o reserva or "Cor all be contracted guaran yer	onclusive or and/or k r, Tribunal tee during	ignant and assend all moresaid a ext, received and bird between and the current arther a external arther a	to the signs) nonies at any course nding, n the ator or rrency

The Employer shall have the fullest liberty, without affecting in any way the liability of the Bank under this guarantee, from time to time to extend the time for performance

of the Contract or the Component Agreement by the O&M Partner. The Employer shall have the fullest liberty, without affecting this guarantee, to postpone from time to time the exercise of any powers vested in them or of any right which they might have against the O&M Partner and to exercise the same at any time, in any manner, and either to enforce or to forbear to enforce any covenants, contained or implied, in the Contract or Undertaking or any other course or remedy or security available to the Employer. The Bank shall not be released of its obligations under this presents by any exercise of its liberty with reference to the matters aforesaid or any of them or by reason of any other act or forbearance or other acts of omission or commission on the part of the Employer or any other indulgence shown by the Employer or by any other matter or thing whatsoever which under law would, but for this provision have the effect of relieving the Bank from its obligations.

The Bank also agrees that the Employer at is option shall be entitled to enforce this Guarantee against the Bank as a principal debtor, in the first instance without proceeding against Contractor or O&M Partner and notwithstanding any security or other guarantee that the Employer may have in relation to Contractor's or O&M Partner's liabilities.

@...... and shall be extended from time to time for

such period (not exceeding one year), as m	· ·
(O&M Partner) on whose behalf this guarantee I	nas been given.
This guarantee shall be valid for one year afte from the date of expiry of O& M period (i.e. 5 `	-
Date this day of	2021 at
WITNESS:	
(Signature)	(Signature)
(Name)	(Name & Designation)
(Official Address)	(Bank's Seal)
	Authorised vide Power of
	Attorney No
	Date
Brief Name of the Contractor	

@ The date will be ninety (90) days after the end of the defect liability period as	
specificed in Contract.	
NOTE:	

- 1. The stamp papers of appropriate value shall be purchased in the name of the Guarantee issuing Bank.
- 2. (i) The Bank Guarantee from a Bank in the list of Banks at Attachment 15 to Section III of bid documents.

MONTHLY FIELD CHECK LIST OF (To be filled by MPCB officials deputed) MCAAQMV UNDER OPERATION CONTRACT ----- (name of the city)

S. No.	Description	(name of the Station) Station	Remarks
1.	Station Visit Date		
	(i) 1st Week		
	(ii) 2 nd Week		
	(iii) 3 rd Week		
	(iv) 4 th Week		
2.	SOP Available at Station		
3.	Environmental Condition of Station		
4.	Protocol of Station available		
5.	Availability of Calibration Gas		
6.	Availability of Permeation Tube (NIST Traceable)		
7.	Bi Weekly Calibration Done (Precision check, two Point calibration check)		
8.	Full Calibration Done (Multipoint Calibration check)		
9.	Insurance Validity		
10.	Electricity Bill Paid, if any		
11.	Telephone Bill Paid, if any		
12.	Security Guard Payment, if any		
13.	Servicing of ACs Installed, if any		

14.	Data Display Board Working	
15.	O&M Rate - Cheque payment, if any	
16.	Name of the Company Engineer Deputed/Present	
17.	Data Analyst at Central Station Deputed/Present	
18.	Log-Book maintained and observation entered.	
19.	Date Received (Daily / Monthly)	
20.	Name of the visiting Official of MPCB	
21.	Special Remarks, if any	

...

Signature of MPCB official

Annexure- X2

Maharashtra Pollution Control Board Continuous Ambient Air Quality Monitoring Report (MAIN POLLUTANTS)

To be submitted daily at 06 morning for that day ending at next 06 morning

!	Daily Re	eport					Stat	ion Nar	ne:		Month:			
I	Report	No.:										Date:	 .	
I	Monito	ring L	ocatio	on:										
1	Data In	iterval	: 1 Hr.	. Aver	age									
I	Monito	ring C	ondu	cted E	By:									
14-15 Hr.														
15-16 Hr.														
16-17Hr.														
17-18 Hr.														
18-19 Hr.														
Hrs.	NO	NO2	NOX	NH3	SO2	СО	О3	PM2.	PM10	Benzen	Toluene	Ethyl Ben	MP	0
								5		е			Xylene	xylene
	µg/m	μg/m	ppb	ug/m	µg/m³	μg/m	µg/m³	µg/m	µg/m	µg/m³	µg/m³	µg/m³	µg/m³	µg/m³
	3	3		3		3		3	3					
19-20 Hr.														
20-21 Hr.														
21-22 Hr.														
22-23 Hr.														
23-00 Hr.														
00-01 Hr.														
01-02Hr.														
02-03 Hr.														
03-04Hr.														
04-05 Hr.					-									
05-06 Hr.														
MINIMUM														
MAXIMUM														
AVERAGE														
Data														
Captured	I			1		1								

Annexure-X3

Maharashtra Pollution Control Board
Continuous Ambient Air Quality Monitoring
Report
(Mean Concentration of Main Pollutants)
Year
Monitoring Location:

Months	NO	NO2	NOX	NH3	SO2	co	03	PM2.5	PM10	Benzen e	Toluene	Ethyl Ben	MP Xylen	O xyler
	µg/m	µg/m³	ppb	μg/m	μg/m	µg/m³	µg/m³	μg/m³	µg/m³	μg/m³	µg/m³	μg/m³	μg/m³	μg/
January														
February														
March														
April -							-							
May														
June														
July														
•														
August														
Septembe	;													
October														
Novembe							-							
Decembe							-							


MINIMUM MAXIMUM AVERAGE

<u>Calculation of City-wise Payment for O & M Charges on Quarterly Basis for MCAAQMV under O & M Contract</u>

Bill raised for O & I					Invoice No.		
Total Amount	es and consumad	nes		II	nvoice No.		
Name of the Statio	n 🗆	STATIC	NI I (Location	STATIO	N II (Location	STATION	l III/I ocation
Quarter No.:) <u> </u>	STATIC	IN I (LOCATION	STATIO	VII (LOCALIOII	STATION	V III (LOCALIOI
Duration:							
Year:							
	Month 1						
valid	Month 2						
monthly data							
captured rate	Month 3						
Average Quarterly Rate □	Data Captured						
		Price for service portion 70%	Price for material part & other incidental charges 30%	Price for service portion	Price for material part & other incidental charges	Price for Service portion	Price for material part & other incidental charges
Base Amount per NoA)(A)	Quarter (as per						
Formula: see	ptured Rate (B) at footnote* culation sheet						
Applicable Dedupenalty provision non-functioning(C) Calculation sheet Annexure II)	for continuous (Specimen						
Any Other Deduct justification(D)	ion, specify with						
Applicable Taxes Service Tax - Ed Secondary &Hig Cess - CST	ducation Cess -						
Net Amount Payal (C+D) +E]	ole (`) [F = B-						
Total O&M cost F Wise)	Payable(Station	(i)		(ii)		(iii)	1
Total Amount Pa	yable (`) for O&	M cost fo	r City for quart	er no	(l +	- ii + iii)	

Note: Separate sheet need to be incorporated for the scheduled Maintenance of the Mobile Vehicle.

(Ref.: Invo	oice nodated	for the period		Annexure I
Name of Station*	Name of non - functional system	Total period of continuous non-functioning (days)	Period considered for penalty calculation after grace period**	Penalty amount (period x unit rate)
	alty Amount (`): be prepared & submitte	ed separately for each	station)	
** Gra	ace period of 7 days is a	pplicable only once p	er quarter	

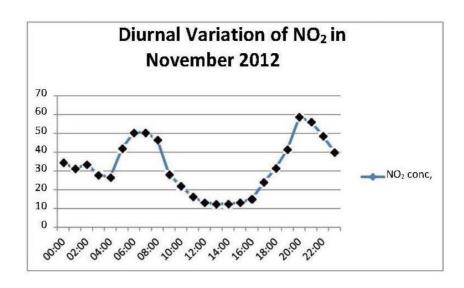

Diurnal Variation of O₃ in November 12

Si

Annu

Diurnal Variation of O₃ in November 12

O₃ conc,

O₃ conc,

O₃ conc,

O₄

O₅


O₆

O₇

O₈

O

ns with

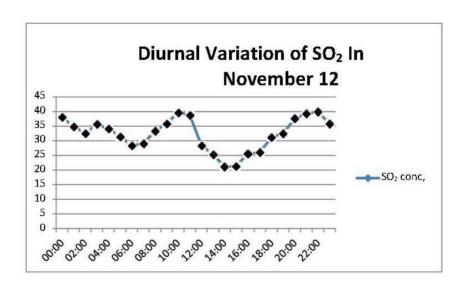

TECHNICAL SPECIFICATIONS FOR

CONTINUOUS REAL TIME AMBIENT AIR QUALITY MONITORING ANALYSERS /

STATION

VOLUME-II

Maharashtra Pollution Control Board

Kalpataru Point, 3rd Floor, Opp. CinePlanet,

Near Sion Circle, Sion (East), Mumbai - 400 022

Tel: 24020781/24010437, Fax: 24023516

website:http://www:mpcb.gov.in

Email Id: jdair@mpcb.gov.in

SCHEDULE OF REQUIREMENTS

The equipments are intended for one Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV). The system should be completely functional. Any balance of material not specified but required for the purpose must be supplied by the vendors.

Schedule	Brief Description	Qty. in Nos.
No.		
1.	Continuous Automatic Air Quality Monitoring Analysers for CO, SO ₂ , NO-NO2-NOx, O3 and BTX	1 Unit each
2.	Automatic PM ₁₀ Monitor	1 Unit each
3.	Automatic PM _{2.5} Monitor	1 unit each
4.	Multi-calibration systems for gaseous monitors comprising of gas SUPPLY / generation and automated calibration	1 Unit each
5.	Sensor Based Meteorological Instrumentation comprising Wind Direction, Wind Speed, Ambient Temperature, Relative Humidity, Solar Radiation and Rain Fall mounted on Telescoping Crank- up Meteorological Tower.	1 unit each
6.	Computer System consisting of one PC and DAS at monitoring Van and one high end PC (Intel core i7 8 th generation processor, 32 GB RAM.2 TB HD,DVD Writer,, HDMI port, COM Port, parallel port must be present on Motherboard. Windows 10 Pro 64 Bit operating system, Colour Printer with Scanner, LED monitor (20 inches – 900 x 1600 resolution) at central office with peripherals and software for data acquisition / display / transfer and system along with Modem and Router.	1 Lot each
7.	2 Ton Capacity Split Air conditioner	2 Units each
8.	Arrangements like Thermally Stable Housing (Body Built up) for installation of Continuous Ambient air quality Monitoring analysers with Sampling line, Internal fitting, Instruments racks, Electrical and Gas line Fittings, Tools (electrical and mechanical).	1 Unit each
9.	Petrol Generator set-10 KVA	1 Unit each
10	Vehicle model number TATA LPT 709Ex 2 or its equivalent, BS-VI variant along with vehicle frame (Chassis build up) air conditioned and thermally stable instrument cabin.	1 Unit each

TECHNICAL SPECIFICATIONS

1.0 MOBILE MONITORING VAN

1.1 Specification of the Vehicle:

Engine Type	TATA 497 TCIC (Bharat Stage-VI)-4 Cylinder, Turbo- intercooled common rail direct injection engine or equivalent
Displacement /Cubic Capacity	3783cc
Max. Power output	93.2KW (125 PS) at 2400 r/min
Max. torque	400Nm @ 1300-1500 r/min
Bore x Stroke	97mm X 128mm
Clutch	Single plate dry friction type-310 mm dia
Transmission	GBS 550 Synchromesh 6Forward & 1 Reverse
Fuel Injection System	In-line type with double plunger and Double cam lobe (CB18-MICO)
Fuel tank capacity (in litres)	160L
Battery	12V, 100 Ah capacity
Alternator	65 Amps
Gradeability	39%- 3400 Wheelbase, 36%- 3800 Wheelbase
Max speed in Top gear (in Kmph)	101 km/h

1.2 Dimensions of the Chassis- Thermally Stable Housing (Body Builtup)

Inside minimum length: Approx. 4200 mm
Inside minimum width: Approx. 3500mm
Inside minimum height: Approx. 2500 mm

- Frame: All the material used for the construction of the floor, frame, roof frame 1.3 etc, the 4 corner posts and 8 integrated, reinforced container corners should be of metal. The exterior panel of the container shall be made of pre-coated MS Sheet of approved colour shade. All other steel parts should be hot dipped galvanized having minimum rate of galvanisation of 275 gram per square meter. All joints of like metal such as steel-tosteel or aluminium-to-aluminium shall be protected against corrosion by liberal application of joining compound. All joints of dissimilar metals such as steel to aluminium shall be protected against corrosion due to galvanic action by liberal application of dielectric compound as well as jointing compound on both mating surfaces. For liftina fixing the container. International Standard eyebolts should be provided at the corners.
- 1.4 Panelling: The outer panelling will be of 1.2 mm of Pre-coated MS sheet to withstand external impacts and abrasions. Outer side of the MS Sheet i.e. exposed face of the sheet, shall be permanently colour coated with silicon modified polyester coating of dry film thickness (DFT) 20 micron (min.) of approved colour shade over primer. Inner face of the sheet shall be provided with suitable pre-coating of minimum 7micronoff-white colour. The inner panelling will be of PVC coated 2 mm thick aluminium sheet, fixed over an inlay of 4 mm marine plywood. 100 mm thick polyurethane insulation will be used between the outer and inner walls (Pre-coated MS sheet and Marine plywood) as insulating material. Z spacers if required shall be made out of at least 2mmthick galvanized steel sheet of grade 275 as per IS:277
- **1.5** Floor: The floor will be laid in frame of 600×600 mm centre to centre with $50 \times 50 \times 6$ mm MS angle. The floor surface will be of 19 mm marine plywood covered with robust quality Vinyl flooring, 2 mm thick of approved colour. The floor should be of

acid and alkaline resistant, waterproof, easily cleanable / washable. Bottom plate of thickness 2 mm hot dipped galvanised MS Plate shall be provided.

- **1.6** Outer Door: One door of size approx. 2000 x 900 mm will be provided at the front side (L = 4200 mm) of the station with isolated 3 point locking & door handle flush fitted.
- 1.7 Electric Power SUPPLY Box: Single- phase (1 Ø) electrical wiring will be laid in ducts. Copper wiring of appropriate gauge will be used. The terminal board should be mounted in a central power distribution box. Over voltage protection for each phase shall be provided along with the lightning arrestor. 2 numbers Emergency cut off switch &Thermostat switch (35° C) for power disconnection, 6 free sockets and 3 fluorescent lamps for lighting will be provided. The station shall be properly grounded with chemical earthing or as per BIS Standards with proper plate and only copper strip at-least on 2 corners (diametrically opposite). One energy meter (Digital Type) shall be installed. Weatherproof cubicles / enclosure for housing of MCB / TP & N Switch of main power termination (outside shelter) and weather proof telephone junction box for terminations of telephone line are to be provided. Proper earthing for telescopic mast of meteorological system shall be provided. There should be conduction between the telescopic mast of the meteorological system and the station. The guy ropes or wires shall be provided for supporting the mast.

List of Consumables:

All Fuses : 02 set Lightning arrestor : 02 set Emergency Switch : 02 pcs Thermostat : 01 pc

1.8 The housing will be partitioned as per drawing to create space for storing of gas Cylinders, Meteorological mast. The minimum size will be $2000 \times 1400 \times 2300$ mm. A lockable door of minimum size 900×2000 mm along-with 3 - Point locking system shall be provided on the outer wall of the housing. A 300 mm, single-phase (230×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 200×100 mm, single-phase (200×100 volts and 20

Air conditioners shall be mounted on proper rust proof supporting structures with rubber blocks to avoid vibration of structures. Proper caging / grill should also be provided for the safety of ACs. Sun shades for external AC units shall be provided with fabricated pre-coated MS sheet (same as monitoring station) with supporting arrangements. AC unit's external piping shall be placed in GI trays. Cable trays fixed on exterior wall shall be covered with pre-coated MS sheet, of same colour shade of monitoring station. Roof top sheet to be levelled and sloped properly. Rain water spout shall be fixed at top with rain water down pipe at two corners. The external lights of the station should be **Solar operated**.

1.9 Station Furnishing:

- (i) 19" or suitable racks 2 or 3 Nos.
- (ii) Fire extinguishers 2 Nos.
- (iii) Furniture:
 - A) Material Furniture made of water resistant laminated board
 - B) Cupboard As per drawing
 - C) Working table Powdered coated MS frame size 1400 x 900 x 750 mm (w x d x h) and top 19 mm thickness Board
 - D) Revolving tilting chair 2 Nos.

(iv) Miscellaneous

- The exhaust gases from the analyser should be collected and a) discharged by a common exhaust pipe and vented.
- b) Thermostat for measuring the temperature of the station
- Hygro Meter for measurement of Humidity inside the station c)
- d) No smoking stickers
- Vacuum cleaner of reputed make with minimum 100 watt power e)
- f) Tool Kit having following tools:
 - 1. One screw driver set
 - 2. One multi-meter (Philips, Mico make)
 - 3. One box spanner set
 - 4. One D spanner set
 - 5. One watch maker set
 - 6. One Hammer set
 - 7. One precision screw driver set
 - 8. One pliers set
 - 9. One Tong tester
- g) One Emergency LED Cluster light
- h) Sign boards along-with logo of Maharashtra Pollution Control Board, to be embedded with suitable size on the side of the van, The name of the Station i.e. Mobile Continuous Ambient Air Quality Monitoring Van, (Location) both in English and Hindi or local language to be inscribed.

2.0 **AIR CONDITIONER**

- 2.1 Type: 2 Nos. split type, with an automatic timer. Separate Voltage stabilizer will be provided with each unit.
- 2.2 Capacity: 2.0 Ton (2 Nos.). The indoor units should be running alternately at an interval of four hours with timer control and the temperature inside the station should be maintained at 25° C inside during peak summer months.
- 2.3 Nominal Cooling: Btu /hr - 24000, Kcal / hr: 6000
- 2.4 Fan type: Propeller Fan
- 2.5 Fan Motor type: Permanent Split Capacitor, 1/8 Horse power
- 2.6 Control Type: Remote
- 2.7 Compressor: Reciprocating
- 2.8 Refrigerant: Eco Friendly
- 2.9 Power Supply: 230 volts \pm 10 volts AC and 50 Hz \pm 3%.

AIR QUALITY ANALYSIS SYSTEM 4.0

(CO, SO₂, NOx, BTX, PM₁₀, and PM_{2.5})

(General Specifications for all Analysers)

- **4.1** The analysers should be 19" rack mounting model with facilities for fixing the analysers from front side.
- 4.2 The ON / OFF switch and display of the entire important status signal viz. Sample flow, temperature, concentration, range switch, manual / auto mode, zero / span mode should be on front panel.
- 4.3 The analysers should operate at operating voltage 230 volts ± 10 volts AC and 50 Hz
 - ± 3%. The power SUPPLY input to be protected against spikes from and to the analyser by an LC filter. The power connection cable should be CEE type complete with 15 Amperes plug adaptable to Indian mains socket.
- 4.4 The analysers must function properly in Indian conditions without any defect between 0 50° C ambient temperature, 10 95% relative humidity and in high ambient dust levels. The data capture rate should not be less than 90%.
- 4.5 The Manufacturer shall provide minimum of 2 weeks of operational & preventive maintenance hands-on training for 3 persons (maximum) per State.
- 4.6 The analysers should be complete with calibration system. The calibration system should be delivered along-with respective span gas cylinder and permeation tubes. The span gas concentration should be within 60 90% of first measuring range. The analyser must have zero point internal calibration system and in agreement with minimum detection limit of each analyser. The calibration procedures are to integrated into the software system for automatic calibration.
- The permeation tube and the calibration gases provided with the system shall have Traceability to NIST.
- 4.8 The analysers shall be supplied with all ancillaries necessary for operation including external pump (if any) and any other items such as charcoal scrubber, Teflon air sample intake filter, drier, Teflon tubing suitable for connection to air sampling manifold. All such items are to be itemized. Dust filter in all the analysers should be provided before solenoid valve to protect frequent chocking of solenoid valve.
- 4.9 The connector systems for out-going signal for recording and the computer terminal should be on back panel with screw type connecting pins.
- 4.10 All ambient gas analysers shall conform with the USEPA automated reference / TUV / EN or equivalent method designation as required by the specification for individual equipment / parameters. Method of measurement used shall also comply with the stipulation on National Ambient Air Quality Standards (NAAQS) 2009 (Details of Methods of Measurement is available at MoEF and CPCB websites). All analysers shall be micro processor controlled with automatic calibration using an external dilution calibrator and calibration standards. All analysers and sensors should be fully integrated in the rack cabinet, fully calibrated & tested before SUPPLY and ready for start up at the respective sites. Analyzer must exhibit performance equal to or better than values specified in the Calibration & test certificate provided with each analyzer.
- **4.11** The manufacturer shall specify the cross sensitivity of measurement for all the analysers.
- **4.12** Each set of analysers shall be supplied with two copies of elaborate operation manuals comprising details in three parts:
 - Parts (I) should comprise installation, operational and trouble shooting details;
 - Parts (II) should have details about preventive, routine and corrective maintenance:
 - Parts (III) should comprise details of all electrical, electronic and pneumatic circuit diagrams, details of each spare parts, Catalogue No. etc. and details of each electronic card / PCB's; and

Parts (IV) Schematic diagram for possible repair & maintenance.

4.13 Digital Output:

a) RS 232/ Ethernet port shared between Analysers, Dust Monitor (PM2.5& PM10), Meteorological Sensors and computer for data, status and control.

4.14 Quality Control and Standard

Data shall be collected and validated according to US EPA standards, using the methodologies included in 40 Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design.

The supplier shall submit a Standard Operating Procedure for the air quality monitoring Vans to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The Standard Operating Procedure shall contain the following:

- i. Operating procedures for all analysers and meteorological sensors
- ii. Calibration procedures
- iii. Calibration schedule
- iv. Maintenance procedures
- v. Maintenance schedule
- vi. Data validation procedures
- vii. Quality Assurance procedures
- viii. Sample quality assurance documentation
- ix. Sample Air Quality Report

The calibration procedures for analysers shall conform to US EPA methodologies and shall include daily calibration checks, biweekly precision checks and linearity checks every six weeks. All analysers shall undergo full calibration every six weeks. Data obtained from these calibration checks and copies of associated Quality Assurance and calibration documentation, shall be submitted to the Buyer along with the Air Quality Data.

Air Quality Data shall be submitted to the Buyer on a monthly basis in the form of an Air Quality Report. This report shall include tabular and graphic information on gas and dust concentrations as well as meteorological data for each site. The

data shall be reported in the form of 15 minute averages and shall also include daily, weekly and monthly averages, minimums, maximums, standard deviations, total data captured and percent data capture. The Air Quality Report shall also include wind roses where wind speed and direction are measured. Upon 24 hour notice from the Buyer, once per year, the supplier shall agree to submit to an audit of calibrations, conducted, using pre-approved US EPA methodologies, by a third party. The results of these audits shall be made immediately available to both the supplier and Buyer.

5.0 SPECIFICATIONS OF SAMPLING SYSTEM

A suitable sampling system as specified by USEPA having 10 ports manifold and fitted with a suction pump to draw ambient air. System duly equipped with moisture removal systems should be provided for sampling of ambient air separately for gaseous and dust measurement.

Gases sampling system:

5.1 Height of the sampling system: Approx. 1.0 meter above the roof

5.2 Roof entry cut out: Stainless Steel
5.3 Conduit: Stainless Steel
5.4 Inner sampling system: Borosilicate glass
5.5 Sampling head: Stainless Steel

5.6 Manifold: 10 port for tubes 6 x 1 mm, self- tightening

6.0 SPECIFICATIONS OF RACK

Suitable sized Rack cabinet to accommodate all analysers, calibrators, Zero air generators, data logger etc. The dimension of the rack without doors, with aluminium section and rear of 2 mm steel sheet, one removable roof plate, fitted with 4 filling eyebolts. Four roof fixing screws included in package to replace the lifting eyebolts. One gland plate three part, one pair of suitable size mounting angles depth adjustable in 25 mm pitch pattern fitted on two fixing angles approximately 150 mm unit from the front standard. To accommodate panel width of 19" size: width = 600 mm, Height = 1400 mm and Depth = 800 mm. The 19" racks should be screwed to the floor of the station with anti-vibration pads. All nuts and bolts shall be cadmium coated.

7.0 AMBIENT AIR QUALITY MONITOIRNG ANALYSERS

(A) AMBIENT OXIDES OF NITROGEN (NO-NO2-NOx) ANALYSER Conforming to USEPA Automated Federal Reference Method (FRM) Designation

01.	Principle	:	Chemiluminescence
02.	Measurement	:	NO / NO2 / NOx in Ambient Air
03.	Display	:	Digital
04.	Ranges	:	Auto ranging 0-2000 PPB
05.	Minimum Detectable Limit	:	1 PPB
06.	Noise Level	:	0.5 PPB
07.	Zero Drift	:	< 1 PPB/24 Hrs.
08.	Span Drift	:	< 2% in 15 days of full scale
09.	Response Time	:	30 seconds or earlier
10.	Linearity	:	± 1% of full scale
11.	Calibration	:	Please see Multi-calibration section (SI. No. J) and also calibration section in General Specifications (4.6 & 4.7).
12.	Output Signals or Analog Output	:	3 Analog output 0 - 1 V, 0 - 10 V, 0 - 20 mA or 4 - 20 mA
13.	Digital Output	:	RS 232 port/ Ethernet

(B) AMBIENT SULPHUR DIOXIDE (SO2) ANALYSER Conforming to USEPA Automated Federal Equivalent Method (FEM) Designation

01.	Principle	:	Pulsed UV Fluorescence	
02.	Measurement	:	Sulphur Dioxide in Ambient Air	
03.	Lower Detectable Limit	:	1 PPB	
04.	Ranges	:	Auto ranging 0 - 500 PPB	
05.	Display		Digital	
06.	Noise Level		0.50 PPB or 1% of the reading	
07.	Zero Drift	:	< 1 PPB / 24 Hrs. With automatic zero	
			compensation	
08.	Span Drift	:	< 2 PPB full scale in 15 days	
09.	Calibration	:	Please see Multi-calibration section (Sl. No.	
			J) and also calibration section in General	
			Specifications (4.6 & 4.7).	
10.	Precision	:	0.5 ppb or 1% reading whichever is greater	
11.	Output Signals or Analog	:	3 Analog output 0 - 1 V, 0 - 10 V, 0 - 20 mA or 4 -	
	Output		20 mA	
12.	Digital Output	:	RS 232 port/ Ethernet	

(C) AMBIENT CARBON MONOXIDE (CO) ANALYSER Conforming to USEPA Automated Federal Reference Method (FRM) Designation

01.	Principle	:	Non Dispersive Infra-Red (NDIR) with Gas Filter Correlation
02.	Measurement	:	Carbon Monoxide in Ambient Air
03.	Display	:	Digital
04.	Ranges	:	At least four ranges Auto ranging 0 - 100 PPM.
05.	Minimum Detectable Limit	:	0.1 PPM
06.	Zero Noise	:	0.05 PPM with time constant ± 30 seconds
07.	Zero Drift	:	< 0.2 PPM/7 days
08.	Span Drift	:	< 1% full scale in 24 hrs.
09.	Calibration	:	Calibration gas (CO) cylinder - 10 liters capacity. A Highly polished aluminum cylinder portable filled with 40 PPM NIST traceable Calibration gas has to be provided along-with the instrument for calibration purpose. It should also have pressure gas valve for Zero and Span gas.
10.	Linearity	:	Continuous + 1%
11.	Output Signals or Analog Output	:	3 Analog output 0 - 1 V, 0 - 10 V, 0 - 20 mA or 4 - 20 mA
12.	Digital Output	:	RS 232 port/ Ethernet

(D) Technical specifications of "AMBIENT OZONE (O3) ANALYSER" Conforming to USEPA Automated Federal Reference Method (FRM) Designation

01	Principle	:	UV Photometric
02	Measurement	:	Ozone in Ambient Air
03	Display	:	Digital
04	Range	:	Auto ranging 0 - 500 PPB
05	Minimum Detectable Limit	:	2.0 PPB
06	Noise	:	± 1.0 PPB
07	Zero Drift	:	< 1/2% per month
08	Span Drift	:	< 1% per month
09	Calibration	:	With built in Zero and span generator and also see Multi-calibration section
10	Linearity	:	Continuous + 1%
11	Output Signals or	:	3 Analog output 0 - 1 V, 0 - 10 V, 0 - 20 mA or
	Analog Output		4 - 20 mA
12	Digital Output	:	RS 232 port/ Ethernet

(E) PM10 MONITOR Conforming to USEPA Automated Federal Equivalent Method (FEM) Designation

Based on the principle of β -ray attenuation by particulate sampled through the instrument and collected on fiberglass filter tape. Before and after sampling β -ray radiation is measured by scintillation / G.M. counter. An internal microprocessor handles all sequences and automatically calculates the concentration of SPM.

01. Principle : Continuous measurement of PM10 in ambient

02. Particle Size Cut Off : air

03. Measuring Range : 0 - 10 Microns
 04. Resolution : 0 to 2000 μg/m³

05. Minimum Detectable: 1% of the concentration

Limit $2 \mu g/m^3$

06. Detector :

Plastic Scintillator / GM Counter, Silicon

07. Air Flow Rate : Semiconductor Beta Detector

08. Filter Material : At - least 1.5 m³ / hrs. (Adjustable to 1 m³/hr)

09. Display : Glass Fiber Filter

10. Sampling Head : LED / LCD

Dynamic heated sampling head for measurement of RM10, with adjustable temporature 20, 70.00

11. Calibration : of PM10, with adjustable temperature 20 - 70 °C

Reference membrane facility should be

12. Compatibility : provided for calibration of analyser.

Analyser should be compatible with protocols

13. Roll Length : mentioned in DAS section14. Measurement Result : Approximately 30 meters

1 hr average or shorter

(F) PM_{2.5} MONITOR Conforming to USEPA Automated Federal Equivalent Method (FEM) Designation

Based on the principle of β -ray attenuation by particulate sampled through the instrument and collected on fiberglass filter tape. Before and after sampling β -ray radiation is measured by scintillation / G.M. counter. An internal microprocessor handles all sequences and automatically calculates the concentration of SPM.

01. Principle : Continuous measurement of PM2.5 in ambient

02. Particle Size Cut Off : air

03. Measuring Range : 0 - 2.5 Microns
 04. Resolution : 0 to 1000 μg/m³

05. Minimum Detectable: 1% of the concentration

Limit $2 \mu g/m^3$

06. Detector :

Plastic Scintillator / GM Counter, Silicon

07. Air Flow Rate : Semiconductor Beta Detector

08. Filter Material : At - least 1.5 m³ / hrs. (Adjustable to 1 m³/hr)

09. Display : Glass Fiber Filter

10. Sampling Head : LED / LCD

Dynamic heated sampling head for measurement

11. Calibration : of PM2.5 with adjustable temperature 20 - 70 °C

Reference membrane facility should be

12. Compatibility : provided for calibration of analyser.

Analyser should be compatible with protocols

13. Roll Length : mentioned in DAS section

Approximately 30 meters

14. Measurement Result : 1 hr average or shorter

Or

(G) Ambient Particulate Monitor based on the principle "Tapered Element Oscillating Microbalance" (TEOM) Conforming to USEPA Automated Federal Equivalent Method (FEM) Designation (EQPM-0609-182)

SPECIFICATIONS

TEOM 1405-DF Ambient Particulate Monitor 1405DF = Dual TEOM w/ FDMS

Regulatory Designations

- U.S. EPA approved PM-2.5 equivalent monitor (EQPM-0609-182)
- Menu-driven software for user interaction via 1/4 VGA display with touch screen
- Connecting and Interface Cables, and Vacuum Pump
- Consumables for average three year's operation (ambient)
- RPCOMM and ePort Software for Local or Remote Communication

Instrument Performance (3 I/min, 1s, stable conditions)

- Measurement Range: 0 to 1,000,000 μg/m³ (1 g/m³)
- Resolution: 0.5 µg/m³
- Precision: ±2.0 μg/m³ (1-hour average), ±1.0 μg/m³ (24-hour avg.)
- Accuracy for Mass Measurement: ±1%

Data Averaging and Output

- Real-time Mass Conc. Average: 1 hour rolling average updated every six minutes
- Long-Term Averaging: 1, 8, and 24 hr
- Data Output Rate: selectable from 10 sec to 24 hour

Operating Range

The temperature of the sampled air may vary between-40 and 60 °C. The TEOM Sensor and Control Units must be weather protected within the range of 8 to 25 °C. An optional Complete Outdoor Enclosure provides complete weather protection.

Sample Flow

- Activol flow control system uses the mass flow sensors and the measured ambient temperature and pressure to maintain constant volumetric flow rates.
- Main Flow Rate: Fine PM filter: 3.0 l/min; Coarse PM filter: 1.67 l/min
- Bypass Flow Rate: 12.0 I/min

(H) Technical specifications of "5 KVA Stabilizer"

01	Installation	:	Wall mount / Table-Top	
02	Display	:	Seven Segment	
03	Operation	:	Automatic	
04	Cabinet Material	:	Metal	
05	Listing Description	:	Automatic Voltage Stabilizer	
			Input Voltage: 90V-300V Application-5KVA/15A Mainline	
06	Input Voltage Range	:	90V-300V	
07	Accuracy	:	±9% or better	
08	Other	:	Cut off protectionOverload-Short circuit protectionSurge protection	

Data Storage

Internal data logging of user-specified variables; capacity of 500,000 records.

Filter Media

- Sample Filter: Pallflex TX40, 13 mm effective diameter
- Sample Conditioner Filter: 47 mm diameter housed in an FRM-style molded filter cassette, maintained at 4°C. Suitable for collecting and archiving time-integrated PM samples for subsequent laboratory analysis.

Sample Conditioning

- Sample Equilibration System (SES) dryer lowers the main flow relative humidity and allows for mass transducer operation at 5°C over the peak air monitoring station temperature
- Purge Filter Conditioner contains a heat exchanger that maintains the temperature of the main flow and particle filter at 4°C to efficiently filter the volatile and non-volatile PM in the sample.

Data Output and Input

- e-Port software to view and change system operation from PC
- Touch screen user interface
- Ethernet with embedded FTP server, USB, RS232, RS485
- 8 User-Defined Analog Outputs (0-1 or 0-5 VDC)
- 2 User-Defined Contact Closure Alarm Circuits
- 4 Averaged Analog Inputs (0-5 VDC) with user-defined conversion to engineering units

(I) BTX MONITOR / ANALYSER

1.0 GENERAL

A complete monitor / analyzer system including continuous automatic sampling (pump etc.), sampling, analyzer, detector, calibrator, computer hardware and software for instrument control, data storage, display, acquisition, processing and for selective determination of volatile compounds in ambient air optimized for Benzene, Toluene, Ethyl Benzene and o, m, p -Xylenes. Compatible to power SUPPLY(voltage 230 volts \pm 10 volts AC and 50 Hz \pm 3%). Continuous unattended measurement system of individual BTEX should work without cryogenic cooling. System should have protocol compatible to communicate & transfer data to main computer through modem and subsequently to CPCB/MPCB website preferably having features of security, data validation & alarms etc. Raw data storage capacity without erase minimum for three month or more. The system should be delivered with all necessary spares, consumables, tubing etc. for making it functional

2.0 TECHNICAL SPECIFICATIONS

2.1 AUTOMATIC SAMPLING (MONITOR) with Sample volume controlled by thermal mass flow controller (dust protected). Sample flow range may be 20 -100 ml/min or more (adjustable). Sample volume should be between 400 ml - one liter or more of ambient air over a 10-15 min sampling cycle. All sample transfer tubing's should be in stainless steel flow / pressure sensor to be preferred with digital display. Sample volume should be controlled by flow controller (dust protected) with volume measurement saved in memory.

2.2 DETECTOR

Photo Ionization Detector (PID) as per EPA/EU/TUV approved specs, which do not require hydrogen gas. The system should have auto-clean & auto calibration facilities. PID Lamp eV should be 10.6eV. PID sensitivity sensor should be available to check sensitivity.

2.3 MINIMUM SPECIFICATIONS

Lowest detector limit : 0.1 µg/m³ (0.03 ppb) or less for Benzene

(There should be no interferences on Methyl-

cyclopentane, 2, 2, 3 - trimethylbutane, 2, 4 - dimethylpentane, Tetrachloromethane, Cyclohexane, 2, 3 - dimethylpentane, 2 - methylhexane, 3 - ethylpentane, Trichloroethylene, n

- heptane, isooctane with BTX components.)

Temperature Range : 5 - 35°C or more

Measuring Range : 1 - 1000 μg / m³ or better

(0.3 ppb to 270 ppb)

Repeatability: Retention Time: <0.1%

RSD

Typical Cycle Time : Amount : <1.0% RSD

Total Cycle Time should not exceed 15/30 min. approx. i.e. Sample Collection Time - 15 min. approx.

Analytical Time - 15 min. approx.

2.5 CALIBRATIONUNITWITH SPANGAS/INBUILT CALIBRATION WITH/PERMEATION TUBES AND GAS MIXING / DILUTION FACILITY

In Built Calibration/Permeation Tubes Facility in the analyzer with the certified permeation tubes and span or calibration gas mixture (low conc. in ppb range, stable for at-least 6 months) with S.S. container/cylinder, regulators with filters should be provided. Calibration unit having gas flow (approx): 10 ml / min (calibration gas); 1.4-2.0 lit / min (dilution gas) with auto gas selection/dilution option for automatic calibration for ppb level calibration gas (10-30 ppb of individual compound of interest). Manual and software selectable valves for sample, calibration span and blank zero air gases. Dilution factor between 1:50 to 150.

2.6 MEMORY AND CONTROL FACILITIES

Method auto load and system restart after power failure. Methods storage capacity with timed events programs for control of system parameters in permanent memory.

Diagnostics & Fault status; gas SUPPLY(low press). System stability (temperature and sample flow). Detector signal (low) and communication should be in digital form on monitor by LED's & be controlled from computer.

Output signals: Analog 0-1 mV, Serial RS 232 for data intermission and CP-BUS for monitor control from remote. Both digital & analog outputs should be available.

2.7 Hardware/Software(s)

Latest PC with operating system/software. Basic Window based latest software's (English version) consisting instrumental control features as well as data storage, acquisition, processing and handling in desired/customized format including sorting of data (1 / 4 / 8 / 12 / 24 hourly, days wise /date wise reporting as microgram / m³ or ppb (selectable) & averaging, data capture rate s etc.).

Data presentation / graphical & statistical processing & data transfer to Excel including time series, correlation matrix etc. is required.

Communication software with protocol compatible to communicate & transfer data from BTX monitor to central computer through modem (preferably including sample chromatogram) and from central computer to CPCB website preferably having features of security, data validation & alarms etc.

System should have remote access to BTX monitor.

Resident program as well BTX control / monitor user program with monitor startup / off / status, blank / calibration and sample gas measured, fault status, carrier gas if any, and communication errors indications. Updation of response factors automatically after calibration run. Auto tune facility. Raw data storage capacity without erase minimum for three month or more.

(J) MULTICALIBRATION SYSTEM

Calibration system should provide for the calibration of the air quality analysers, data acquisition system, meteorological equipment, and gas calibration system.

a) Gas Calibration System:

The calibration system for air monitoring equipment (listed above) should incorporate an automatic gas dilution calibrator, calibration gas standards and a high performance zero air generator to calibrate all of the analysers in the system. The calibration cycles should be able to be configured through the Data Acquisition System at any specific time during the day and night. It should be mounted on standard 19" rack.

The dilution calibrator should be able to perform mixing of source gas, from the calibration gas bottles, with zero air generator, in order to generate a wide range of calibration gas concentrations and minimising the number of calibration gas standards required. All the calibration gases provided along-with the system MUST be NIST Traceable (certificate should be provided). The system should include at

least three permeation chambers and should accept a Permeation Tube up to 11

cm in total length and 2 cm in diameter. It should also have facility for Gas Phase titration (GPT), having Ozone generator of 6 PPM / Liters and the converter efficiency should be 100 % for conversion of NO2 concentration to NO.

The system should also include calibration of Ozone analyzer.

b) Meteorological, Flow and Electronics Calibration

The supplier should provide calibration devices or calibration check devices for all the meteorological and other electrical equipment mentioned above as per the specifications of the manufacturers.

8.0 METEOROLOGICAL MONITORING SYSTEM

The meteorological instrumentation should be interfaced directly with the Data Acquisition System after passing through a lightning protection isolation box. A

crank

up telescopic 10 meters tower should be erected for mounting of meteorological sensors. The relative humidity and solar radiation sensors should be mounted on the tower. All sensors should be NIST (National Institute for Standards and Technology, USA) traceable. The specifications are follows:

(a) WIND SPEED

Range (Operation) 0 - 60 m/s or better Sustainability Up-to 75 m/sec

Accuracy ± 0.5 m/sec or better

Resolution 0.1 m/sec Sensor Type Ultrasonic 0.5 m/sec or less Threshold Response time : 10 sec or better

WIND DIRECTION (b)

: 0 - 359 degree Range Accuracy : ± 5 degree or better

Resolution : 1 degree Sensor type : Ultrasonic Threshold : 0.5 m/sec or less : 10 sec or better Response time

(c) AMBIENT TEMPERATURE

-10 ° C to 60 ° C Range

± 0.2 ° C or better (with radiation shield) Accuracy

Response 10 seconds in still air Sensor type Resistance type Response time 10 sec or better

(d) RELATIVE HUMIDITY

0 to 100% RH Range Accuracy ± 3.0 % or better

Resolution 1%

Sensor type Capacitive / Solid State

Response Time 10 sec or better

SOLAR RADIATION (e)

0 to 1500 W/m² or better Range

Accuracy ± 5.0 % or better

Resolution 5W/m²

(f) **RAINFALL**

Range 0.2 mm to 100 mm/hr

Accuracy ± 5% or better Resolution 0.2 mmSensor type

Tipping bucket rain gauge or any other suitable

sensor

Response Time : 10 sec or better

(g) TELESCOPIC CRANK - UP METEOROLOGICAL TOWER

The wind speed, wind direction, temperature, relative humidity and solar radiation sensors are to be mounted on the Meteorological Tower. The tower is to be a free standing four section telescopic tower provided with a hand crank to raise and lower the instruments mounted on the tower. Specifications are as follows:

Extended Height : 10 meters Retracted Height : 2 metres

Wind load Limit : 0.7896 sq. m. (8.5 sq. ft) at 50 mph

Number of Sections : 4

Construction material : Galvanised steel or aluminium

Note: Humidity and temperature sensors are to be supplied with weather and thermal radiation shield made of anodized aluminium and sensor should be supplied with all necessary cables, connector and mounting arrangements as required.

(h) SPECIFICATIONS OF DATA LOGGER

Data logger with 8 analog, 24 digital inputs and 18 bit resolution. Ability to log channels at different intervals and should have capability of averaging and displaying real time data and averaged data over a period of 1 min, 10 min, ½ hr, 1 hr, 4 hrs, 8 hrs, 24 hrs, 1 month and year. Communication between data logger and computer using standard multi drop RS 232 Connector. The data logger should have internal battery with charger. The data logger should support PSTN line or Internal GSM modem for data transfer.

9.0 SPECIFICATION OF SOFTWARE FOR MCAAQMV.

TABLE OF CONTENT

- A. DATA ACQUISITION SYSTEM IN THE STATION
- B. DATA ACQUISITION SYSTEM IN THE CENTRAL
- C. COMPATIBILITY
- D. SECURITY
- E. OTHER TECHNICAL CONDITIONS
- **F.** ANNEXURE I DETAILS OF DESIRED DATA VALIDATION SYSTEM
- G. LIST OF PROTOCOLS FOR WHICH SOFTWARE SHOULD SUPPORT
- **H.** CHECKLISTTO COMPARE FIRM'S TECHNICAL CAPABILITY TABLE FOR SPECIFICATION OF SOFTWARE.

A DATA ACQUISITION SYSTEM IN THE STATION

SPECIFICATIONS OF STATION SOFTWARE

The station software captures data from all channels in the system and stores in the Personal Computer. Personal computer is used for calibration and configuration of each channel.

1) Data Acquisition

- a) Frequency of data acquisition
 - i) User selectable 1, 5, 30, 60, 120 second averaging duration online digitally.
- b) Channel size
 - i) 32 Channels or more supported
 - ii) Expandable to 64 channels, if required in future
- c) Data input
 - i) Either Analog (0-1 volt / 0-10 volt / 2-20mA / 4-20mA)
 - ii) Or Digital (firm will develop the protocol, if required without additional cost within project duration) to configure with the PC.
- d) User configurable channels, stations and equipments with communication parameters.
- e) Analyzer data channel should comprise of Name, Units, Communication Address, Validity Range, Operation and Error Status.
- f) Provision to incorporate conversion factors such as PPB to μg/m³ etc.
- g) Software should be equipped to configure the analysers with it, irrespective of the output mode i.e. Analog or Digital (RS 232) of the instrument.
- h) System should read raw data values of the analysers and meteorological instruments and duration of averaging data should be user selectable like 10 / 20 / 30 / 40 / 50 / 60 seconds.
- i) The output should be converted into realistic data in prescribed units.

2) Data Collection

- a) Software should collect each second data.
- b) Average data over user selectable time (1, 5, 30, 60 seconds time interval) period.
- c) Operational status, Error status, calibration status and calibration values observed from the analyzer should be captured and should be made available along with the data with a frequency of maximum five minutes.
- d) System should collect of the diagnostics of the instrument comprising actual diagnostics parameters and their values at least once in every five minute to check the state of the health analyzer.
- e) Calibration parameters
 - i) Provision to entering calibration, span calibration values of gas cylinder/permeation to devices
 - ii) Provision for collecting zero calibration, span calibration values(pre calibration & post calibration) in to the database for further analysis.
 - iii) Provisions to collect electronic system pre calibration & post calibration to ascertain the percentage deviation/ correction apply during each calibration.

3) Data Storage

- a) Data along-with diagnostic, calibration, alarms should be stored at station computer at a defined path.
- b) Interval of data dumping will be same as defined in the data collection
- c) System should be capable to keep every second acquired data from 32

channels for a period of minimum five years.

d) Data stored should be plain text format

e) No data encryption should be done at the station and if encryption is done than decryption procedure should be made available in soft file format to check the data at station at any point of time. To convert data on continuous basis for exporting to any other software, if required, procedure should be available without any licensing.

4) Data Display (Statistical analysis of data)

- a) In 4-in-4 graphs, 4-in-1 graph and / or 16-in-1 graph formats
- b) In terms of 4-in-1 table format
- c) Real time multi graphs over user selectable time period.
- d) Display of graphic & tabular display of the current data.
- e) Graphical form should comprise of 4-4 graphs, 4-1 graphs in user defined formati.e. 1, 5, 10, 15, 30 min, 1hour, 4, 8, 24 hour, 30 days and yearly. (user definable time series)
- f) Tabular form should comprise of 4 channel list in user defined format i.e. 1, 5, 10, 15, 30 min, 1hour, 4, 8, 24 hour, 30 days and yearly. (user definable time series)
- g) Station instruments basic configuration etc. should be visible on screen continuously.
- h) Main window for real time display of all measured parameters with status of all analysers/sensors.
- i) Statistical analysis tools like regression analysis, co-relation analysis and other analysis as per industry standards in the field of environment should be available and if not the firm should develop these for MPCB within a time frame.
- j) The system should have procedures for normal analysis tools like calculation of data with respect to a threshold value, average, minimum, maximum, calculation of violating value with respect defined values (Air Quality Standards) for defined period for the database etc.
- k) Data analysis of diagnostics parameters
- Data analysis of Pre calibration and post calibration data (if facility not available can be developed)
- m) Data analysis of corrections applied of each calibration cycle (if facility not available can be developed)

5) Data Backup

- a) There should be defined data backup procedure through which data can be Extracted from station computer in simple text format / excel (user Definable).
- b) There should be defined restore procedure also to restore the data in case of data loss.
- c) A display screen should be available to update the user about data availability.

6) Data Validation automatic checks at station software

- a) Zero level and span level checks if performed cyclically and defined results are not obtained up to +/- 5% (user definable 0-10%) then system should alarm the user of system failure and the recorded alarm should be transmitted to central software.
- b) After instruments perform the calibration the results obtained should be recorded and should be transmitted to central computer.

7) Data validation requests generated at station computer

At least three tier request generation and request acceptance system procedure is desired. Details are given in the **Annexure -I**.

- a) Inbuilt checks capability may be provided, where if instrument throws erratic data software can check automatically and display message and send information in the form of corrected data in corrected database to be approved by the central software at central level. (facility if not available needs to be developed by the system provider)
- b) There should be provision of two databases one is raw database and another corrected database. (facility if not available needs to be developed by the

system provider)

c) Validation of data through calibration database Pre calibration & post calibration values collected.

8) Calibration of systems

a. Calibration window for analyzer for the calibration from computer.

b.Remote Access to Calibration: Calibration exercise need to be done remotely.

All necessary arrangements for it should be made in the system.

- c.Calibration data file may be prepared separately.
- d.Calibration database need to be formed, stored and transmitted to central.
- e.Calibration cycles to be as per the models of the instruments.
- f. Calibration records should store the calibration values displayed by instrument.
- g.Diagnostics during calibration should also be recorded.

9) Location of station

- a) Fixed Station location to be recorded
- b) Moving station location to be recorded
- c) Latitude and longitude of Vans be recorded

10) Data transfer to Central

All data captured at station computer should be transferred to central software.

- a) User selectable time frame for transmission of data to central server.
- b) Diagnostics (actual diagnostics parameter values recorded each time in the station), configurations (station channel configurations), alarms(generated alarms) should be transmitted.

B DATA ACQUISITION SYSTEMAT THE CENTRAL STATION

SPECIFICATIONS OF CENTRAL SOFTWARE

Data communication system handles the data transmission of an ambient air quality network and receives incoming messages / signals from remotely stationed Vans. The central software processes signals and data and displays it on the web and other interfaces. Detailed requirement is as below:

Software at Central Station

- a) Software should not have any restriction on number of locations and computers either technologically or in terms of licensing.
- b) Should display multiple stationed Vans on line data (momentary values) in tabular

text and graphic format.

- c) Data should be received by the central from all locations within 5minutes duration or at user defined time intervals.
- d) Data along-with diagnostics and calibration details should be transmitted at central from all connected locations.
- e) Should support dialup systems, broadband connectivity, wireless connectivity, 2G or 3G or any new technology which shall be in place during project time should be compatible and if not need to developed by the system provider

up-to project duration without additional charges.

- f) Should have the remote control facilities for calibrations (Zero & Span) of instruments and measuring range modifications.
- g) Should have facility for displaying data communication error reports, image management which should be recorded and should be available for display.

2) Data Display at Central

- a) In 4-in-4 graphs, 4-in-1 graph and/or 16-in-1 graph formats
- b) In terms of 4-in-1 table format
- c) Real time multi graphs over user selectable time period.
- d) Display of graphic & tabular display of the current data like simple 3D line and column chart, polar diagnostics and 3D perspective column chart.
- e) Graphical form should comprise of 4-4 graphs, 4-1 graphs in user defined format i.e. 1, 5, 10, 15, 30 min, 1hour, 4, 8, 24 hour, 30 days and yearly. (user definable time series)
- f) Tabular form should comprise of 4 channel list in user defined format i.e. 1, 5,10, 15, 30 min, 1hour, 4, 8, 24 hour, 30 days and yearly. (user definable timeseries)
- g) Display of data using selectable name of different Vans.
- h) Generation of Wind Roses, Pollution Roses (12 & 16 directional i.e. 0degree, 22.5, 45, 67.5, 90 and 360 degree) with user defined time limits.
- i) Calculate vector mean of wind direction.
- i) Programmable down loading of data.
- k) Comparison of data w.r.t. Standards in Graphical form and tabular form within formation of values exceeds the Standards. I) Specific data zooming facility
- m) Database correction procedure
- n) Separate user ID and Password for correction of database so that all regional level users if authorized can validate their regions data and the events be recorded along-with ID and time.
- o) Data validation trail recording.

3) Data Export

- a) Customizable data format developing capability required.
- b) Possibility to export the data files in Excel, Text and other formats Tabular form should be in user defined format i.e. 1, 5, 10, 15, 30 min, 1 hour, 4, 8, 24 hour, 30 days and yearly.

4) Data Import

a) In case of communication medium phase there should a mechanism to shift the data into Pen drive (Physical medium for data collection) physically and a procedure to import the same on central software.

5) Printing

a) Possibility to connect different types of printers and auto printing facility for all displays generated throughout the analysis of data at any point of time.

6) Data Validation automatic checks at Central software

- a) Zero level and span level checks if performed cyclically and defined results are not obtained up to +/- 5% (user definable 0-10%) then system should generate alarm the user of system failure and the recorded alarm should be transmitted to central software and stored. There should be provisions to read these alarms in a database for corrective actions and for comparison of data for acceptability or rejection.
- b) After instruments perform the calibration the results obtained should be recorded and should be transmitted to central computer and stored.
- c) There should be provisions to configure at least 08 alarms for any given instrument auto check.
- 7) Data validation requests management at central computer (if not available facility may be developed by the firm)
- a) Data validation requests sent by station computer should be recorded and the system should provide a window to user to accept or reject the reasons mentioned by the user end.
- b) Inbuilt checks capability should be provided, which can be configured by the administrator at central to put alarms according to requirement on data, errors generated or on diagnostics of systems.
- c) The software at central should have facility to log in data validation requests. These requests will carry the erroneous data for user selected period and for which user at station will request to change the data due to environmental or instrumental operation conditions. These requests will reside in central location and whenever user at central agrees the data will be changed in the validated database. Hence, system will have two types of databases 1)

Raw

database which can never be touched 2) which has to be modified and corrected as per agreed conditions. The detail of user requesting or applying changes in corrected database should be recorded with time.

7. Data Display at Web (if not available facility may be developed by the firm)

- a) System should have standard web display software in place.
- b) Central software should be capable to show the data in predefined formats at website on a physical map.
- c) The data from Corrected database shall be displayed on the web.
- d) Current data should be displayed on web page.
- e) There should be provisions to show no. of violations occurred, percentage of

violation occurred at stationed Vans parameters comparing hourly, 8 hourly, 24 hourly and yearly standards

- f) Provision is required to change standard value, since standard values do change after certain period of time as per Govt. policy.
- g) Displayed web page should have facility of providing information to all with respect to environment as well as to provide specific files for downloading.
- h) The logo of MPCB should be displayed on webpage.
- i) The disclaimer have to be provided on the webpage
- j) Some predefined queries have to be developed to display the data on webpage. A search page needs to be developed for converting data into meaningful format for the general public.
- k) The current data displayed on the web should have comment inserting facility at individual data and for running data as well like if any station instrument out of order then station official should be able to display message "Instrument under maintenance".

- Similarly, when data goes beyond a defined limit it should automatically display a predefined message as comment on webpage as "Data under Scrutiny".
- m) Automatic e-mail messages to be generated for the identified end users to start a corrective action.
- n) Station photos to be uploaded for the display along-with the data.
- o) User defined 05 pages may be developed additionally, if required by MPCB designs for which may be decided mutually.
- 9) Data display at display board outside the office at central location also
 Data display is also required at regional and central locations for which software
 provision has to be made at each location.

10) Remote Procedures (if not available facility may be developed by the firm)

- a) Central software should have capability to allow to connect any station instrument through remote.
- b) Central software administrator should be able to go for remote calibration of any of the systems.
- c) Software should be capable to operate remotely stationed Vans configurations.
- d) Control panel window should be available for controlling each analyzer.
- e) Alarm window for valid alarms of all analysers and sensors.
- f) It should have transparent data connection to each analyzer from remote.
- g) System should be capable to remotely configure all stationed Vans through remote location using configuration file to maintain the uniformity. The configuration command from central or from regional location should be active.

11) Data Reports Generation

- a) To prepare reports hourly, weekly, monthly, yearly in user defined interval and formats.
- b) Mean, Median, Percentile, Maximum, Standard deviation, Frequency analysis and Maximum Frequency analysis.
- c) System should have predefined user selectable procedures through which
 - reports of any specific or stationed Van reports up to four parameters can be generated as per user selected time frame.
- d) Data Comparison
- Software should be able to compare any of the four channels irrespective of type of data in the system with respect to each other on a single time scale user selectable.
- e) Data Comparison on different time scale
- Software should be able to compare data on the basis of different time scales like one station (x) parameter (y) of one given date is compared with other station (z) parameter (y) on any other date in a single graph.
- f) Data reports, calibration reports and status reports with user time periods.
- g) Historic multi curves / graphs over user selectable time period.
- h) Report generation over user selectable time period (instantaneous or averaged over a period of 1, 15, 30 min, 1 hr, 4, 8, 12, 16 and 24 hrs etc.).
- i) Diurnal variation, standard deviation, regression and other statistical parameter reporting possibilities with various available mathematical methods.
- j) If required separate report generation procedures have to be developed for which firm will be responsible for project duration.

C. Compatibility

Should have compatibility with the latest Operating System with a contract of 05 (five) years from the date of Supply of software for providing assistance to operate system at MPCB and all the new patches developed for the software during these 05 years without additional cost. Software should have capability of data transmission with the presently available PROTOCOL (list attached).

D. Security

- a. System should have the facility to have it Password protected or without password as decided by MPCB at the time of implementation.
- b. System software should be totally secured and any antivirus software required to run the system for the complete project duration has to be managed by the system provider.

E. Other Technical Conditions

- 1. Hardware required for data transmission has to be made available by the firm and there should not be non-compatibility.
- 2. Firm should have the capability to develop the Software PROTOCOL for data transmission from any system available in the field in future during next 05 years or up-to the project period.
- 3. Should support the latest formats of Windows 32 bit or 64 bit or any other available platform like Linux etc.
- 4. Manual of complete system should be provided.
- 5. Firm should provide the hardware required for data acquisition along with all the software's required like OS, MS. Office, Networking software, Remote functionality software, Data uploading software on website, Data display software if required, and should maintain hardware for project duration.
- 6. Since, system has to be placed in NIC domain for which the web software developed along-with the database and web server software should be

certified by CERT-IN empanelled vendors for vulnerability. The system provider is responsible for fulfilling all criteria required to place the system at NIC domain. The firm will be responsible for entire duration of the project for any vulnerability if noticed by NIC.

F. DETAILS OF DESIRED DATA VALIDATION SYSTEM

Annexure-I

At least three tier request generation and requests acceptance procedure are desired in the system. It is presumed that level 1 is station, level 2 is Central location at regional level and level 3 at Central level.

The regional and central levels will have central station computers and software installed and stationed Vans will have station computer installed with station data acquisition software and data transmission software.

The flow of data has to be from stationed Vans to Regional Level and then to Central level. It is desired that environmental database has to be corrected for instrumentation issues as well as for the environmental issues. Hence, officials available at stations will communicate with central and state levels through system itself by commenting on the data. The respective data can be picked up from the database at stationed Vans itself, corrected to the desired numbers and then transmitted to regional level central computer where, the administrator of system if agrees to the changes desired then data flows to the next level else request rejected. If request will come to Central server for accepting or rejecting

then central level should have authority of accepting or rejecting the data. If central level agrees to the changes than data should be changed in the corrected database else request should be rejected. Hence, there should be provisions for accepting or rejecting data at all three levels accordingly. Here, whenever such requests are generated, concerned administrators need to be sent email alerts.

G. List of protocols for which CAAQM software should support


Bayern-Hessen Intercomp 6 LabCom	Intercomp5 Intercomp 1 Metek USA-1	FH62 Konf. PVM100 VC820	ChemPro 100 MultiPD II X am 7000
Unor, Oxor	AK R+P	TSI 30222/25	HG Monitor 3000
Defor Multor Adam Module CLD700 FH62 Hygrowin Gesytec II RFM433 NMEA183	MBF Gemi Uras 14 Modbus Binos1000 HP34970A Almemo Modbus DGH Module BH/Timo 9600	Blendmaster Klimet Thygan USA Turbulence Thies DL14/15 Innova1312 Multiwarn II MeteoBus Windobserver	ESM FH40G Travelpilot DX-V AK Conf. Thermo Instr. PR820R PAC3 Data Collect SDR VDO Navigation

H. Checklist to compare Firm's Technical capability table for specifications of Software


S. No.	Details	Capability of firm's software as on date	Firm agree or disagree to develop software in future	If firm agrees to develop application then time frame from individual activity
1.	Data transfer interval Max. 5 minutes from all locations?			
2.	System will transmit data along with diagnostics. If yes then how many channels diagnostics values shall be transmitted to central and at what duration?			
3.	System will transmit data along with Calibration values (Pre cal and Post Cal)?			
4.	System has remote calibration procedures in place for Regional level and central level both?			
5.	System has remote configuration facility for regional and central level both?			
6.	System has database validation procedure in place?			
7.	Web software already developed or not?			
8.	If Web software is available is it modifiable as per CPCB need by the firm?			
9.	Whether agree to develop five web pages as per mutual discussion			
10.	Web software with password and or without password			
11.	Password providing facility available at regional levels			
12.	Statistical tools available at web software or not?			
13.	System provider is capable of placing system in NIC domain			
14.	System provider will provide certification from CERT-IN empanelled firms			

15.	Data import from other files		
16.	Data export to other files		
17.	Pre defined queries to be inbuilt for providing data to public whether these are already available or to be developed if yes then time frame?		
18.	Standards comparison and exceedances be reported on		
19.	Different types of predefined formats of report preparation available or not?		
20.	support various protocols available till date as listed provided or not?		
21.	If new protocol based software is to be developed whether firm will		
22.	Unlimited Number of stations supported by Central Server software or not? If not then support for how many stations will be provided		
23.	System compatibility with Dialup/BB/2G/3G/Wireless available or not? If not then what technologies supported as on date? What time frame if other to be develop.		
24.	Software has Wind rose reports generating capability		
25.	Software has pollution rose generating facility		
26.	Software has diurnal variation facility		
27.	Software has mathematical tools		
28.	Software has 16 channels display at on page		
29.	Software has data communication error reports		
30.	System has error correction procedure		
31.	Software has parallel data display		

	reports	
32.	Software has virtual channel deployment capacity	
33.	Software has data encrypting procedures at stations or not? If yes then data can be retrieved from station or not?	
34.	Software compatible for ANDROID technology	
35.	System Provider will provide all Hardware required at station and Central	
36.	System Provider all necessary software required for data acquisition, display, Analysis, website uploading etc.	

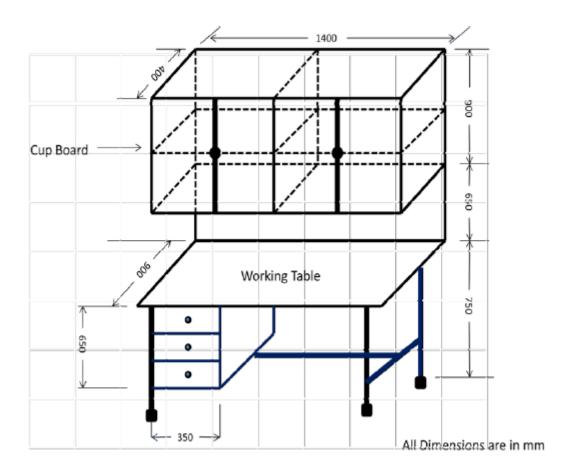

Drawing of Cup Board and Working Table

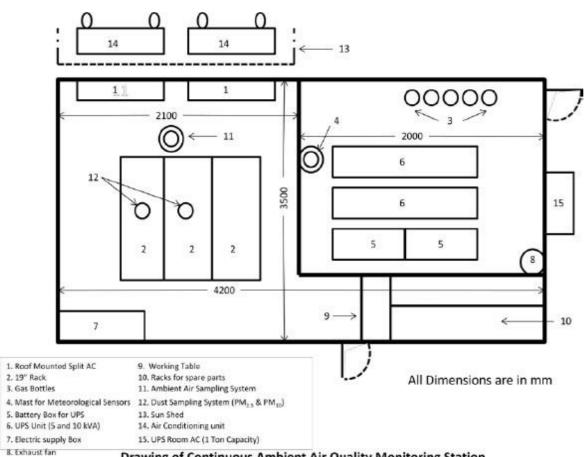

Drawing of Continuous Ambient Air Quality Monitoring Station

E	BLANK	PAGE						
	C	etelleties cod co		datanana	labila Cardinus A 11	and Air Oughter & A. Co.	/on /BACA A CA B A	
	Supply, in:	stallation and commissioni	ng and Operation & ma	untenance services of M	IODIIE CONTINUOUS AMBIE	an Air Quality ivionitoring \	ran (IVICAAQIVIV)	

VOLUME-II MAHARASHTRA POLLUTION CONTROL BOARD

Technical Data Sheet for SUPPLY and O & M of Mobile Continuous Ambient Air Quality Monitoring Van (MCAAQMV)

Sr. No.	Specifications	SUPPLY and O & W of Mobile Continuous Ambie	Bidder's Response
1	MONITORINGS STATION		
1.1	Monitoring Station: To be build up on Chassis of Vehicle model number TATA LPT 709Ex 2 or its equivalent, BS-VI variant	Monitoring Station: is designed for housing the ambient air quality monitoring instruments to protect them from dust and heat. Temperature and Humidity sensors shall be installed in the housing for checking the humidity and temperature inside the station. Three Nos. 19" racks shall be installed inside the station so that the analysers are easily accessible from front & back for calibration and maintenance.	
1.2	Dimensions:	Inside length: Approx. 4200 mm Inside width: Approx. 3500 mm Inside height: Approx. 2500 mm	
1.3	Frame	All the material used for the construction of the floor, frame, roof frame etc, the 4 corner posts and 8 integrated, reinforced container corners should be of metal. The exterior panel of the container shall be made of pre- coated MS Sheet of approved colour shade. All other steel parts should be hot dipped galvanized having minimum rate of 176 galvanization of 275 gram per square meter. All joints of like metal such as steel-to-steel or aluminium-to-aluminium shall be protected against corrosion by liberal application of joining compound. All joints of dissimilar metals such as steel to aluminium shall be	

Sr. No.	Specifications		Bidder's Response
		protected against corrosion due to galvanic action by liberal application of dielectric compound as well as jointing compound on both mating surfaces. For lifting / fixing the container, International Standard eye bolts should be provided at the corners.	
1.4	Panelling	The outer panelling will be of 1.2 mm of Pre- coated MS sheet to withstand external impacts and abrasions. Outer side of the MS Sheet i.e. exposed face of the sheet, shall be permanently colour coated with silicon modified polyester coating of dry film thickness (DFT) 20 micron (min.) of approved colour shade over primer. Inner face of the sheet shall be provided with suitable pre-coating of minimum 7 micron off-white colour. The inner panelling will be of PVC coated 2 mm thick aluminium sheet, fixed over an inlay of 4 mm marine plywood. 100 mm thick polyurethane insulation will be used between the outer and inner walls (Pre- coated MS sheet and Marine plywood) as insulating material. Z spacers if required shall be made out of at least 2 mm thick galvanized steel sheet of grade 275 as per IS:277	
1.5	Floor	The floor will be laid in frame of 600 x 600 mm centre to centre with 50 x50 x 6 mm MS angle. The floor surface will be of 19 mm marine plywood covered with robust quality Vinyl flooring, 2 mm thick of approved colour. The floor should be of acid and alkaline resistant, waterproof, easily cleanable / washable. Bottom plate of thickness 2 mm hot dipped galvanised MS Plate shall be provided.	

Sr. No.	Specifications		Bidder's Response
1.6	Outer Door	One door of size approx. 2000 x 900 mm will be provided at the front side (L = 4200 mm) of the station with isolated 3 - point locking & door handle flush fitted.	
1.7	Electric Power SUPPLY Box	Three - phase (3 Ø) electrical wiring will be laid in ducts. Copper wiring of appropriate gauge will be used. The terminal board should be mounted in a central power distribution box. Over voltage protection for each phase shall be provided along with the lightning arrestor. 2 numbers Emergency cut off switch & Thermostat switch (35° C) for power disconnection, 6 free sockets and 3 fluorescent lamps for lighting will be provided. The station shall be properly grounded with chemical earthing or as per BIS Standards with proper plate and only copper strip at-least on 2 corners (diametrically opposite). One three phase energy meter (Digital Type) shall be installed. Weatherproof cubicles / enclosure for housing of MCB / TP & N Switch of main power termination (outside shelter) and weatherproof telephone junction box for terminations of telephone line are to be provided. Proper earthing for telescopic mast of meteorological system shall be provided. There should be conduction between the telescopic mast of the meteorological system and the station. The guy ropes or wires shall be provided for supporting the mast. List of Consumables All Fuses : 02 set Lightning arrestor: 02 set Emergency Switch: 02 pcs Thermostat : 01 pc	

Sr. No.	Specifications		Bidder's Response
1.8	Housing	The housing will be partitioned as per drawing to create space for storing of gas cylinders, Meteorological mast & UPS. The size will be 2000 x 1400 x 2300 mm. A lockable door of size 900 x 2000 mm along- with 3 - Point locking system shall be provided on the outer wall of the housing. A 300 mm, single-phase (230 volts ± 10 volts AC and 50 Hz ± 3%) exhaust fan with safety grills will be provided. Mounting brackets in 2 levels for fixing of atleast 06 (six) gas bottles should be provided. The internal lights of the housing should be sensor based. Air conditioners shall be mounted on proper rust proof supporting structures with rubber blocks to avoid vibration of structures. Proper caging / grill should also be provided for the safety of ACs. Sun shades for external AC units shall be provided with fabricated pre-coated MS sheet (same as monitoring station) with supporting arrangements. AC unit's external piping shall be placed in GI trays. Cable trays fixed on exterior wall shall be covered with precoated MS sheet, of same colour shade of monitoring station. Roof top sheet to be levelled and sloped properly. Rain water spout shall be fixed at top with rain water down pipe at two corners. The external lights of the station should be Solar operated.	

Sr. No. Spec	ifications		Bidder's Response
1.9 Station Fur	(vi)	Fire extinguishers - 2 Nos. Furniture: e) Material - Furniture made of water resistant laminated board f) Cupboard - As per drawing g) Working table - Powdered coated MS frame size 1400 x 900 x 750 mm (w x d x h) and top 19 mm thickness Board h) Revolving tilting chair - 2 Nos. Miscellaneous h) The exhaust gases from the analyser should be collected and discharged by a common exhaust pipe and vented. i) Folding aluminium ladder for roof access j) Thermostat for measuring the temperature of the station k) Hygro Meter for measurement of Humidity inside the station l) Mounting bracket for the ladder m) No smoking stickers n) Vacuum cleaner of reputed make with minimum 100 watt power h) Tool Kit having following tools: 10. One screw driver set 11. One multi-meter	

Sr. No.	Specifications		Bidder's Response
		(Philips, Mico make) 12. One box spanner set 13. One D spanner set 14. One watch maker set 15. One Hammer set 16. One precision screw driver set 17. One pliers set 18. One Tong tester i) One Emergency LED Cluster light j) Sign boards along-with logo of Central Pollution Control Board, Delhi / State Pollution Control Board, to be embedded with size 1500 x 900 mm on the front of the container and on the two side of the container, The name of the Station i.e. Continuous Ambient Air Quality Monitoring Station, (Location) both in English and Hindi or local language to be inscribed. The Signs boards to be mounted on the station with proper spacers.	
2.0	AIR CONDITIONER		
2.1	Туре	3 Nos. split type, roof mounted of 5 star rating with an automatic timer. Separate Voltage stabilizer will be provided with each unit.	
2.2	Capacity	2.0 Ton (2 Nos.) and 1Ton (1 No.). The indoor units should be running alternately at an interval of four hours with timer control and the temperature inside the station should be maintained at 25° C inside during peak summer months.	
2.3	Nominal Cooling	Btu /hr - 24000, Kcal / hr: 6000	
2.4	Fan type	Propeller Fan	
2.5	Fan Motor type	Permanent Split Capacitor, 1/8 Horse power	
2.6	Control Type	Remote	

Sr.	Specifications		Bidder's Response
2.7	Compressor	Reciprocating	
2.8	Refrigerant	Eco Friendly	
2.9	Power SUPPLY	230 volts ± 10 volts AC and 50 Hz ± 3%.	
3.0	Portable Petrol Generator set- 6.5 kVA		
3.1.1	Capacity	6.5 KVA	
3.1.2	Technology	PWM using IGBT / MOSFETS	
3.1.3	Crest Factor	More than 3: 1	
3.1.4	Input Voltage Voltage Range Frequency	230 V AC ± 25% 50 Hz ± 3%	
3.1.5	Output Voltage Voltage regulation Frequency Frequency regulation Waveform	230 V AC ± 1% 50 Hz ± 0.01% Pure sine wave	
3.1.6	Battery Battery type Back up time Battery Capacity Recharge time	Sealed maintenance free 1 Hour at full load For required backup time 5 hrs to 90% after complete discharge	
3.1.7	Distortion	Less than 1% on linear load	
3.1.8	Power factor	0.9 to 1	
3.1.9	Indicator	L.E.D Battery Charge, Load level, on Line, over load, on battery, replace battery	
3.1.10	Alarm	Audible alarm for batter backup, battery low, and fault	

3.1.11	Protections Surge Overload Short circuit Battery low cut - off	Surge suppression meets BIS or International standard Fuse & current limited Fuse & current limited &cut - off No battery drain after cut - off
3.1.11	Protections	110% for continuous load
3.1.13	Efficiency	More than 90%
3.1.14	EnvironmentOperating Temperature Operating Humidity Audible Noise	0 - 500 C 10% to 95% (Non condensing) Less than 45 db (at 1 meter)
3.2	Single phase 5 KVA Stabilizer along with Automatic Delayed Restoration Device (ADRD) with 2 hours backup in full capacity should be provided for the smooth operation of Analysers and peripherals at the station	
3.2.1	Capacity	5.0 KVA wall maounted or table top mounted
3.2.2	Technology	PWM using IGBT / MOSFETS
3.2.3		More than 3: 1
3.2.4	Input Voltage Voltage Range Frequency	90V-300V ± 25% 50 Hz ± 3%
3.2.5	Output Voltage Voltage regulation Frequency Frequency regulation Waveform	230 V AC ± 1% 50 Hz ± 0.01% Pure sine wave
3.2.6	Battery Battery type Back up time Battery Capacity Recharge time	Sealed maintenance free 2 Hour at full load For required backup time 5 hrs to 90% after complete discharge

3.2.7	Distortion	Less than 1% on linear load	
3.2.8	Power factor	0.9 to 1	
3.2.9	Indicator	L.E.D Battery Charge, Load level, on Line, over load, on battery, replace battery	
3.2.10	Alarm	Audible alarm for batterybackup, battery Low and fault	
Sr. No.	Specifications		Bidder's Response
3.2.11	Protections Surge Overload Short circuit Battery low cut - off	Surge suppression meets BIS or International standard Fuse & current limited Fuse & current limited & cut - off No battery drain after cut - off	
3.2.12	, J	110% for continuous load	
3.2.13		More than 90%	
3.2.14	Operating Temperature Operating Humidity Audible Noise	0 - 500 C 10% to 95% (Non condensing) Less than 45 db (at 1 meter)	
4.0	AIR QUALITY ANALYSIS SYSTEM		
	(CO, SO2, NOx, NH3, BTX, PM10, PM2.5 and O3 Analysers) (General Specifications for all Analysers)		
4.1	The analysers should be 19" rack mounting model with facilities for fixing the analysers from front side		
4.2	The ON / OFF switch and display of the entire important status signal viz. Sample flow, temperature, concentration, range switch, manual / auto mode, zero / span mode should be on front panel.		

4.3	The analysers should operate at operating voltage 230 volts ± 10 volts AC and 50 Hz ± 3%. The power SUPPLY input to be	
Sr. No.	Specifications	Bidder's Response
	protected against spikes from and to the analyser by an LC filter. The power connection cable should be CEE type complete with 15 Amperes plug adaptable to Indian mains socket.	
4.4	The analysers must function properly in Indian conditions without any defect between 0 - 500 C ambient temperature, 10-95% relative humidity and in high ambient dust levels. The data capture rate should not be less than 90%.	
4.5	The Manufacturer shall provide minimum of 2 weeks of operational & preventive maintenance hands-on training for 3 persons (maximum) per State.	

4.6	The analysers should be complete with calibrations system. The calibration systems should be delivered along-with respective span gas cylinder and permeation tubes. The span gas concentration should be within 60 - 90% of first measuring range. The analyser must have zero point internal calibration system and in agreement with minimum detection limit of each	
Sr. No.	Specifications	Bidder's Response
	analyser. The calibration procedures are to integrated into the software system for automatic calibration.	
4.7	The permeation tube and the calibration gases provided with the system shall have Traceability to NIST.	
4.8	The analysers shall be supplied with all ancillaries necessary for operation including external pump (if any) and any other items such as charcoal scrubber, Teflon air sample intake filter, drier, Teflon tubing suitable for connection to air sampling manifold. All such items are to be itemized. Dust filter in all the analysers should be provided before solenoid valve to protect frequent chocking of solenoid valve.	

4.9	The connector systems for outgoing signal for recording and the computer terminal should be on back panel with screw type connecting pins.	
4.10	All ambient gas analysers shall conform with the USEPA automated reference / TUV /EN or equivalent method designation as required by the specification for individual equipment / parameters.	

Method of measurement used shall also comply with the stipulation on National Ambient Air Quality Standards (NAAQS)2009 (Details of Methods of Measurement is available at MoEF and CPCB websites). All analysers shall be micro -processor controlled with automatic calibration using an external dilution calibrator and calibration standards. All analysers and sensors should be fully integrated in the rack cabinet, fully calibrated &tested before SUPPLY and	Sr. No.	Specifications	Bidder's Response
ready for start - up at the respective sites. Analyzer must exhibit performance equal to or better than values specified in the Calibration & test certificate provided with each analyzer.		shall also comply with the stipulation on National Ambient Air Quality Standards (NAAQS)2009 (Details of Methods of Measurement is available at MoEF and CPCB websites). All analysers shall be micro -processor controlled with automatic calibration using an external dilution calibrator and calibration standards. All analysers and sensors should be fully integrated in the rack cabinet, fully calibrated &tested before SUPPLY and ready for start - up at the respective sites. Analyzer must exhibit performance equal to or better than values specified in the Calibration & test certificate provided with	

	T	
4.11	The manufacturer shall specify the cross sensitivity of measurement for all the analysers.	
4.12	Each set of analysers shall be supplied with two copies of elaborate operation manuals comprising details in three parts: Parts (I) should comprise installation, operational and	
Sr. No.	Specifications	Bidder's Response
	trouble shooting details; Parts (II) should have details about preventive, routine and corrective maintenance; Parts (III) should comprise details of all electrical, electronic and pneumatic circuit diagrams, details of each spare parts, Catalogue No. etc. and details of each electronic card / PCB's; and	
	Parts (IV) Schematic diagram for possible repair & maintenance.	

4.13	Digital Output: a)RS 232/ Ethernet port shared between Analysers, Dust Monitor (PM2.5 & PM10),Meteorological Sensors and computer for data, status and control.	
4.14	·	

Sr.	Charifications	Bidder's Response
No.	Specifications	•

methodologies included in 40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration schedule xiii. Maintenance procedures xiv. Maintenance schedule xv. Data validation procedures xvi. Quality Assurance procedures xvii. Sample quality assurance documentation	Sr.	Specifications	Bidder's Response
ACOODE of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration procedures xiii. Maintenance procedures xiv. Maintenance schedule xv. Data validation procedures xvi. Quality Assurance procedures xvi. Quality Assurance procedures xvii. Sample quality assurance			<u> </u>
ACOODE of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration procedures xiii. Maintenance procedures xiv. Maintenance schedule xv. Data validation procedures xvi. Quality Assurance procedures xvi. Quality Assurance procedures xvii. Sample quality assurance			
ACOde of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration procedures xiii. Maintenance procedures xiv. Maintenance schedule xv. Data validation procedures xvi. Quality Assurance procedures xvi. Quality Assurance procedures xvii. Sample quality assurance			
ACOde of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration procedures xiii. Maintenance procedures xiv. Maintenance schedule xv. Data validation procedures xvi. Quality Assurance procedures xvii. Sample quality assurance		dodinonation	
AlCode of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The Standard Operating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration procedures xiii. Maintenance procedures xiv. Maintenance schedule xv. Data validation procedures xvi. Quality Assurance yrocedures xvi. Quality Assurance yrocedures			
All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration schedule xiii. Maintenance schedule xiii. Maintenance schedule xv. Data validation procedures xvi. Quality Assurance			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration schedule xiii. Maintenance procedures xiv. Maintenance schedule xv. Data validation procedures			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration schedule xiii. Maintenance procedures xiv. Maintenance schedule		•	
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration schedule xiii. Maintenance procedures			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures xii. Calibration schedule			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors xi. Calibration procedures			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all analysers and meteorological sensors			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following: x. Operating procedures for all		meteorological sensors	
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the following:			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating Procedure shall contain the			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to award. The StandardOperating			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be approved by the Buyer prior to			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This Standard Operating Procedure shall be		approved by the Buyer prior to	
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time of bid submission. This		Operating Procedure shall be	
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring stations to the Buyer at the time			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure for the air quality monitoring			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a Standard Operating Procedure			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall be of the latest design. The supplier shall submit a			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall			
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent method designation and shall		j – j	
40Code of Federal Regulations. All analysers shall have current US EPA reference or equivalent			
40Code of Federal Regulations. All analysers shall have current			
40Code of Federal Regulations.			
40Code of Federal			
المناه والمواجع		methodologies included in	

Specifications

No.

submitted to the Buyer along with the Air Quality Data. Air Quality Data shall be submitted to the Buyer on a monthly basis in the form of an Air Quality Report. This report shall include tabular and graphic information on gas and dust concentrations as well as meteorological data for each site. The data shall be reported in the form of 15 minute averages and shall also include daily, weekly and monthly averages, minimums,	
---	--

	maximums, standard deviations, total data captured and percent data capture. The Air Quality Report shall also include wind roses where wind speed and direction are measured. Upon 24 hour notice from the Buyer, once per year, the supplier shall agree to submit to an audit of calibrations, conducted, using preapproved US EPA methodologies, by a third party. The results of these audits shall be made immediately available to both the supplier and Buyer.		
5.0	SPECIFICATIONS OF SAMPLING SYSTEM		
	A suitable sampling system as specified by USEPA having 10ports manifold and fitted with a suction pump to draw ambient air. System duly equipped with moisture removal systems should be provided for sampling of ambient air separately for gaseous and dust measurement. Gases sampling system:		
5.1	Height of the sampling system:	Approx. 1.0 meter above the roof	
5.2	Roof entry cut out:	Stainless Steel	

Sr. No.	Specifications		Bidder's Response
5.3	Conduit:	Stainless Steel	
5.4	Inner sampling system:	Borosilicate glass	
5.5	Sampling head:	Stainless Steel	
5.6	Manifold:	10 port for tubes 6 x 1 mm, self- tightening	
6.0	SPECIFICATIONS OF 19" RACK Suitable 19" Rack cabinet to accommodate all analysers, calibrators, Zero air generators, data logger etc. The dimension of the rack without doors, with aluminum section and rear of 2mm steel sheet, one removable roof plate, fitted with 4 filling eyebolts. Four roof fixing screws included in package to replace the lifting eyebolts. One gland plate three part, one pair of 475mm (19") mounting angles depth adjustable in 25 mm pitch pattern fitted on two fixing angles approximately 150 mm unit from the front standard. To accommodate panel width of19" size: width = 600 mm, Height= 1400 mm and Depth = 800mm. The 19" racks should be screwed to the floor of the station with anti-vibration pads. All nuts and bolts shall be cadmium coated.		
7.0	AMBIENT AIR QUALITY MONITOIRNG ANALYSERS		
(A)	AMBIENT OXIDES OF NITROGEN (NO-NO2-NOx) ANALYSER		

Sr. No.	Specifications		Bidder's Response
	Conforming to USEPA		
	Automated Federal Reference Method		
1.	Principle	Chemiluminescence	
2.	Measurement	NO / NO2 / NOx in Ambient Air	
3.	Display	Digital	
4.	Ranges	Auto ranging 0-2000 PPB	
5.	Minimum Detectable Limit	1 PPB	
6.	Noise Level	0.5 PPB	
7.	Zero Drift	< 1 PPB/24 Hrs.	
8.	Span Drift	< 2% in 15 days of full scale	
9.	Response Time	30 seconds or earlier	
10.	Linearity	± 1% of full scale	
11.	Calibration	Please see Multi-calibration section (Sl.	
		No. J) and also, calibration section in `	
		General Specifications (4.6 & 4.7).	
12.	Output Signals or Analog Out	3 Analog output 0 - 1 V, 0 - 10 V, 0 - 20 mA	
	put	or 4 - 20 mA	
13.	Digital Output	RS 232/ Ethernet port	
(C)	AMBIENT SULPHUR DIOXIDE (SO2)		
	ANALYSER Conforming to USEPA		
	Automated Federal Equivalent		
	Method (FEM) Designation	5 1 110/5	
1.	Principle	Pulsed UV Fluorescence	
2.	Measurement	Sulphur Dioxide in Ambient Air	
3.	Lower Detectable Limit	1 PPB	
4.	Ranges	Auto ranging 0 - 500 PPB	
5.	Display	Digital	
6.	Noise Level	0.50 PPB or 1% of the reading	
7.	Zero Drift	< 1 PPB / 24 Hrs. With automatic zero	
8.	Span Drift	compensation	
	Span Drift	< 2 PPB full scale in 15 days	
9.	Calibration	Please see Multi-calibration section (Sl. No.	
		J) and also, calibration section in General	
		Specifications (4.6 & 4.7).	

Sr. No.	Specifications		Bidder's Response
10.	Precision	0.5 ppb or 1% reading whichever is greater	
11.	Output	3 Analog output 0 - 1 V, 0 - 10 V, 0 - 20 mA or 4 - 20 mA	
12.	Digital Output	RS 232/ Ethernet port	
(D)	AMBIENT OZONE (O3) ANALYSER Conforming to USEPA Automated Federal Reference Method (FRM) Designation		
1.	Principle	UV Photometric	
2.	Measurement	Ozone in Ambient Air	
3.	Display	Digital	
4.	Range	Auto ranging 0 - 500 PPB	
5.	Minimum Detectable Limit	2.0 PPB	
6.	Noise	± 1.0 PPB	
7.	Zero Drift	< ½% per month	
8.	Span Drift	< 1% per month	
9.	Calibration	With built in Zero and span generator and also see Multi-calibration section (Sl. No. J)	
10.	Linearity	Continuous + 1%	
11.	Output Signals or Analog Output	3 Analog output 0 - 1 V, 0 - 10 V, 0 - 20 mA or 4 - 20 mA	
12.	Digital Output	RS 232/ Ethernet port	
(E)	AMBIENT CARBON MONOXIDE (CO) ANALYSER Conforming to USEPA Automated Federal Reference Method (FRM) Designation		

Sr. No.	Specifications		Bidder's Response
01.	Principle	Non-Dispersive Infra-Red (NDIR) with Gas Filter Correlation	
02.	Measurement	Carbon Monoxide in Ambient Air	
03.	Display	Digital	
04.	Ranges	At least four ranges Auto ranging 0 - 100 PPM.	
05.	Minimum Detectable Limit	0.1 PPM	
06.	Zero Noise	0.05 PPM with time constant ± 30 seconds	
07.	Zero Drift	< 0.2 PPM/7 days	
08.	Span Drift	< 1% full scale in 24 hrs.	
09.	Calibration	Calibration gas (CO) cylinder - 10 litres capacity. A Highly polished aluminium cylinder portable filled with 40 PPM NIST traceable Calibration gas has to be provided along-with the instrument for calibration purpose. It should also have pressure gas valve for Zero and Span gas.	
10.	Linearity	Continuous + 1%	
11.	Output Signals or Analog Output	3 Analog output 0 - 1 V, 0 - 10 V, 0 - 20 mA or 4 - 20 mA	
12.	Digital Output	RS 232/ Ethernet port	
(F)	PM10 MONITOR Conforming to USEPA Automated Federal Equivalent Method (FEM)Designation Based on the principle of β-ray attenuation by particulate sampled through the instrument and collected on fiberglass filter		

Sr. No.	Specifications		Bidder's Response
	tape. Before and after sampling β-ray radiation is measured by scintillation / G.M. counter. An internal microprocessor handles all sequences and automatically calculates the concentration of SPM.		
01.	Principle	Continuous measurement of PM10 in ambient air	
02.	Particle Size Cut Off	0 - 10 Microns	
03.	Measuring Range	0 to 2000 μg/m ³	
04.	Resolution	1% of the concentration	
05.	Minimum Detectable Limit	2 μg/m ³	
06.	Detector	Plastic Scintillator / GM Counter, Silicon Semiconductor Beta Detector	
07.	Air Flow Rate	At - least 1.5 m ³ / hrs. (Adjustable to 1 m ³ /hr)	
08.	Filter Material	Glass Fibre Filter	
09.	Display	LED / LCD	
10.	Sampling Head	Dynamic heated sampling head for measurement of PM10, with adjustable temperature 20 - 70 °C	
11.	Calibration	Reference membrane facility should be provided for calibration of analyser.	
12.	Compatibility	Analyser should be compatible with protocols mentioned in DAS section	
13.	Roll Length	Approximately 30 meters	
14.	Measurement Result	1 hr average or shorter	
(G)	PM2.5 MONITOR Conforming to USEPA Automated Federal Equivalent Method (FEM)		

Sr. No.	Specifications		Bidder's Response
	Designation		
	Based on the principle of β -ray attenuation by particulate sampled through the instrument and collected on fiberglass filter tape. Before and after sampling β -ray radiation is measured by scintillation / G.M.counter. An internal microprocessor handles all sequences and automatically calculates the concentration of SPM.		
01.	Principle	Continuous measurement of PM2.5 in ambient	
02.	Particle Size Cut Off	0 - 2.5 Microns	
03.	Measuring Range	0 to 1000 μg/m³	
04.	Resolution	1% of the concentration	
05.	Minimum Detectable Limit	2 μg/m³	
06.	Detector	Plastic Scintillator / GM Counter, Silicon	
	A. E.	Semiconductor Beta Detector	
07.	Air Flow Rate	At - least 1.5 m ³ / hrs. (Adjustable to 1 m ³ /hr)	
08.	Filter Material	Glass Fiber Filter	
09.	Display	LED / LCD	
10.	Sampling Head	Dynamic heated sampling head for measurement of PM2.5 with adjustable temperature 20 - 70 °C	
11.	Calibration	Reference membrane facility should be provided for calibration of analyser.	
12.	Compatibility	Analyser should be compatible with protocols mentioned in DAS section	
13.	Roll Length	Approximately 30 meters	
14.	Measurement Result	1 hr average or shorter	

Sr. No.	Specifications		Bidder's Response
	Or		
(H)	Ambient Particulate Monitor based on the principle "Tapered Element Oscillating Microbalance" (TEOM) Conforming to USEPA Automated Federal Equivalent Method (FEM) Designation (EQPM-0609-182		
	SPECIFICATIONS		
	TEOM 1405-DF Ambient Particulate Monitor 1405DF = Dual TEOM w/ FDMS		
	Regulatory Designations	 •U.S. EPA approved PM-2.5 equivalent monitor (EQPM-0609-182) •Menu-driven software for user interaction via 1/4 VGA display with touch screen •Connecting and Interface Cables, and Vacuum Pump •Consumables for average three year's operation (ambient) •RPCOMM and ePort Software for Local or Remote Communication 	
	Instrument Performance (3 I/min, 1s, stable conditions)	 Measurement Range: 0 to 1,000,000 μg/m³ (1 g/m³) Resolution: 0.5 μg/m³ Precision: ±2.0 μg/m³ (1-hour average), ±1.0 μg/m³ (24-hour avg.) 	

Sr. No.	Specifications		Bidder's Response
	Data Averaging and Output	 Real-time Mass Conc. Average: 1 hour rolling average updated every six minutes Long-Term Averaging: 1, 8, and 24 hr Data Output Rate: selectable from 10 sec to 24 hour 	
	Operating Range	 The temperature of the sampled air may vary between-40 and 60 °C. The TEOM Sensor and Control Units must be weather protected within the range of 8 to 25 °C. An optional Complete Outdoor Enclosure provides complete weather protection. 	
	Sample Flow	 Activol flow control system uses the mass flow sensors and the measured ambient temperature and pressure to maintain constant volumetric flow rates. Main Flow Rate: Fine PM filter: 3.0 l/min; Coarse PM filter: 1.67 l/min Bypass Flow Rate: 12.0 l/min 	
	Data Storage	 Internal data logging of user-specified variables; capacity of 500,000 records. 	
	Filter Media	 Sample Filter: Pallflex TX40, 13 mm effective diameter Sample Conditioner Filter: 47 mm diameter housed in an FRM-style molded filter cassette, maintained at 4°C. Suitable for collecting and archiving time-integrated PM samples for subsequent laboratory analysis. 	
	Sample Conditioning	 Sample Equilibration System (SES) dryer lowers the main flow relative humidity and allows for mass transducer operation at 5°C over the peak air monitoring station 	

Sr. No.	Specifications		Bidder's Response
		temperature • Purge Filter Conditioner contains a heat exchanger that maintains the temperature of the main flow and particle filter at 4°C to efficiently filter the volatile and non-volatile PM in the sample.	
	Data Output and Input	 ePort software to view and change system operation from PC Touch screen user interface Ethernet with embedded FTP server, USB, RS232, RS485 8 User-Defined Analog Outputs (0-1 or 0-5 VDC) 2 User-Defined Contact Closure Alarm Circuits 4 Averaged Analog Inputs (0-5 VDC) with user-defined conversion to engineering units 	
(I)	BTX MONITOR / ANALYSER	ongino onnig annie	
1.0			

Sr. No.	Specifications	Bidder's Response
	Benzene and o, m, p -Xylenes. Compatible to power SUPPLY UNDER BUY-BACK(voltage 230 volts ± 10 volts AC and 50 Hz ± 3%). Continuous unattended measurement system of individual BTEX should work without cryogenic cooling. System should have protocol compatible to communicate & transfer data to main computer through modem and subsequently to CPCB/MPCB website preferably having features of security, data validation & alarms etc. Raw data storage capacity without erase minimum for three month or more. The system should be delivered with all necessary spares, consumables, tubing etc. for making it functional	
2.0	TECHNICAL SPECIFICATIONS	
2.1	AUTOMATIC SAMPLING (MONITOR) with Sample volume controlled by thermal mass flow controller(dust protected). Sample flow range may be 20 - 100 ml/min or more (adjustable). Sample volume should be between 400ml - one liter or more of ambient air over a 10-15 min sampling cycle. All sample	

Sr. No.	Specifications		Bidder's Response
	transfer tubing's should be in stainless steel flow / pressure sensor to be preferred with digital display. Sample volume should be controlled by flow controller (dust protected) with volume measurement saved in memory.		
2.2	DETECTOR Photo Ionization Detector (PID)Asper EPA/EU/TUV approved specs, which do not require hydrogen gas. The system should have auto- clean & autocalibration facilities. PID Lamp eV should be 10.6eV. PID sensitivity sensor should be available to check sensitivity.		
2.3	MINIMUM SPECIFICATIONS		
	Lowest detector limit	0.1 µg/m³ (0.03 ppb) or less for Benzene(There should be no interferences on Methyl-cyclopentane,	
	Temperature Range	5 - 35°C or more	
	Measuring Range	1 - 1000 μg / m³ or better (0.3 ppb to 270 ppb)	
	Repeatability	Retention Time : <0.1% RSD Amount : <1.0 % RSD	

Sr. No.	Specifications		Bidder's Response
	Typical Cycle Time	Total Cycle Time should not exceed 15/30min. approx. i.e. Sample Collection Time -15 min. approx. Analytical Time - 15 min. approx.	
2.5	CALIBRATION UNIT WITH SPAN GAS / IN BUILT CALIBRATION WITH /PERMEATION TUBES AND GAS MIXING / DILUTION FACILITY In Built Calibration/Permeation Tubes Facility in the analyzer with the certified permeation tubes and span or calibration gas mixture (low conc. in ppb range, stable for at-least 6months) with S.S. container/cylinder, regulators with filters should be provided. Calibration unit having gas flow(approx): 10 ml / min(calibration gas); 1.4-2.0 lit / min(dilution gas) with auto gas selection/dilution option for automatic calibration for ppb level calibration gas (10-30 ppb of individual compound of interest). Manual and software selectable valves for sample, calibration span and blank zero air gases. Dilution factor between 1:50 to 150.		
2.6	MEMORY AND CONTROL FACILITIES		

Sr. No.	Specifications	Bidder's Response
	Method auto load and system restart after power failure. Methods storage capacity with timed events programs for control of system parameters in permanent memory. Diagnostics & Fault status; gas SUPPLY(low press). System stability (temperature and sample flow). Detector signal(low) and communication should be in digital form on monitor by LED's & be controlled from computer. Output signals: Analog 0-1 mV, Serial RS 232 for data intermission and CP-BUS for monitor control from remote. Both digital & analog outputs should be available.	
2.7	Hardware/Software(s) Latest PC with operating system/software. Basic Window based latest software's (English version) consisting instrumental control features as well as data storage, acquisition, processing and handling in desired/customized format including sorting of data (1 / 4 /8 / 12 / 24 hourly, days wise/date wise reporting as microgram / m3 or ppb(selectable) & averaging, data	

Sr. No.	Specifications	Bidder's Response
	capture rate s etc.) Data presentation / graphical & statistical processing & data transfer to Excel including time series, correlation matrix etc. is required.	
	Communication software with protocol compatible to communicate & transfer data from BTX monitor to central computer through modem (preferably including sample chromatogram) and from central computer to CPCB website preferably having features of security, data validation & alarms etc. System should have remote access to BTX monitor. Resident program as well BTX control / monitor user program with monitor start-up / off / status, blank / calibration and sample gas measured, fault status, carrier gas if any, and communication errors indications. Updation of response factors automatically after calibration run. Auto tune facility. Raw data storage	
	capacity without erase minimum for three month or more.	

Sr. No.	Specifications	Bidder's Response
(J)	MULTICALIBRATION SYSTEM	
	Calibration system should	
	provide for the calibration of	
	the air quality analysers, data	
	acquisition system,	
	meteorological equipment, and	
	gas calibration system.	
a)	Gas Calibration System:	
	The calibration system for air	
	monitoring equipment (listed	
	above) should incorporate an	
	automatic gas dilution	
	calibrator, calibration gas	
	standards and a high	
	performance zero airgenerator	
	to calibrate all of the analysers	
	in the system. The calibration	
	cycles should be able to be	
	configured through the Data	
	Acquisition System at any	
	specific time during the day	
	and night. It shouldbe	
	mounted on standard 19" rack.	

The dilution calibrator should be able to perform mixing of source gas, from the calibration gas bottles, with zero air generator, in order to generate a wide range of calibration gas concentrations and minimising the number of calibration gas standards required. All the calibration gases provided along-with the system MUST be NIST Traceable (certificate should be provided). The system should include at least three permeation chambers and should accept a Permeation Tube up to 11 cm in total length and 2 cm in diameter. It should also have facility for Gas Phase titration (GPT), having Ozone generator of 6 PPM / Liters and the converter efficiency should be 100 % for conversion of NO2 concentration to NO.

Sr. No.	Specifications	Bidder's Response
	The system should also include calibration of Ozone analyzer.	
b)	Meteorological, Flow and Electronics Calibration The supplier should provide calibration devices or calibration check devices for all the meteorological and other electrical equipment mentioned above as per the specifications of the manufacturers.	

Sr. No.	Specifications		Bidder's Response
8.0	METEOROLOGICAL MONITORING		
	SYSTEM		
	The meteorological		
	instrumentation should be		
	interfaced directly with the		
	Data Acquisition System after		
	passing through a lightning		
	protection isolation box. A		
	crank - up telescopic 10 meters		
	tower should be erected for		
	mounting of meteorological		
	sensors. The relative humidity		
	and solar radiation sensors		
	should be mounted on the		
	tower. All sensors should be		
	NIST		
	(National Institute for Standards		
	and Technology, USA) traceable. The specifications		
(0)	WIND SPEED		
(a)	_	0 - 60 m/s or better	
	Range (Operation)		
	Sustainability	Up-to 75 m/sec ± 0.5 m/sec or better	
	Accuracy		
	Resolution	0.1 m/sec	
	Sensor Type	Ultrasonic	
	Threshold	0.5 m/sec or less	
(1.)	Response time	10 sec or better	
(b)	WIND DIRECTION	0.050.1	
	Range	0 - 359 degree	
	Accuracy	± 5 degree or better	
	Resolution	1 degree	
	Sensor type	Ultrasonic	
	Threshold	0.5 m/sec or less	
	Response time	10 sec or better	

Sr. No.	Specifications		Bidder's Response
(c)	AMBIENT TEMPERATURE		
	Range	-10 ° C to 60 ° C	
	Accuracy	± 0.2 ° C or better (with radiation shield)	
	Response	10 seconds in still air	
	Sensor type	Resistance type	
	Response time	10 sec or better	
(d)	RELATIVE HUMIDITY		
	Range	0 to 100% RH	
	Accuracy	± 3.0 % or better	
	Resolution	1%	
	Sensor type	Capacitive / Solid State	
	Response Time	10 sec or better	
(e)	SOLAR RADIATION		
	Range	0 to 1500 W/m ² or better	
	Accuracy	± 5.0 % or better	
	Resolution	5W/m ²	
(f)	RAINFALL		
	Range	0.2 mm to 100 mm /hr	
	Accuracy	± 5% or better	
	Resolution	0.2 mm	
	Sensor type	Tipping bucket rain gauge or any other suitable sensor	
	Response Time	10 sec or better	
(g)	TELESCOPIC CRANK - UP METEOROLOGICAL TOWER The wind speed, wind direction, temperature, relative humidity and solar radiation sensors are to be mounted on the Meteorological Tower. The tower is to be a free standing four section telescopic tower provided with a hand crank to		

Sr. No.	Specifications		Bidder's Response
	raise and lower the instruments		
	mounted on the tower.		
	Specifications are as follows:		
	Extended Height	10 meters	
	Retracted Height	2 metres	
	Wind load Limit	0.7896 sq. m. (8.5 sq. ft) at 50 mph	
	Number of Sections	4	
	Construction material	Galvanised steel or aluminium	
	Note: Humidity and		
	temperature		
	sensors are to be supplied with weather and		
	thermal radiation shield made of		
	anodized aluminium and sensor		
	should be supplied with all		
	necessary cables, connector		
	and		
(h)	SPECIFICATIONS OF DATA		
	Data logger with 8 analog, 24		
	digital inputs and 18 bit		
	resolution. Ability to log		
	channels at different intervals		
	and should have capability of		
	averaging and displaying real		
	time data and averaged data		
	over a period of 1 min, 10 min,		
	1/2 hr, 1 hr, 4 hrs, 8 hrs, 24 hrs, 1		
	month and year.		
	Communication between data logger and computer using		
	standard multi drop RS 232		
	Connector. The data		
	logger		
	should have internal battery		

Sr. No.	Specifications	Bidder's Response
	should support PSTN line	
	or Internal GSM modem for data	
9.0		
9.0	MCAAQMV.	
	TABLE OF CONTENT	
	I. DATA ACQUISITION SYSTEM	
	IN THE STATION	
	J. DATA ACQUISITION SYSTEM	
	IN THE CENTRAL	
	III III OLIVIIO L	
	K. COMPATIBILITY	
	I OFOURITY	
	L. SECURITY	
	M.OTHER TECHNICAL	
	CONDITIONS	
	N. ANNEXURE - I	
	DETAILS OF DESIRED DATA VALIDATION SYSTEM	
	VALIBATION OF OTEN	
	O. LIST OF PROTOCOLS FOR	
	WHICH SOFTWARE SHOULD	
	SUPPORT	
	P. CHECKLIST TOCOMPARE	
	FIRM'S TECHNICAL	
	CAPABILITY TABLE FOR	
	SPECIFICATION OF	
	SOFTWARE.	

Sr. No.	Specifications		Bidder's Response
A	DATA ACQUISITION SYSTEM IN THE STATION SPECIFICATIONS OF STATION SOFTWARE The station software captures data from all channels in the system and stores in the Personal Computer. Personal computer is used for calibration and configuration of each channel.		
1)	Data Acquisition	c) Frequency of data acquisition i) User selectable 1, 5, 30, 60, 120 second averaging duration online digitally. d) Channel size i) 32 Channels or more supported ii) Expandable to 64 channels, if required in future e) Data input i) Either Analog (0-1 volt / 0-10 volt / 2- 20mA / 4-20mA) ii) Or Digital (firm will develop the protocol, if required without additional cost within project duration) to configure with the PC. f) User configurable channels, stations and equipments with communication parameters. g) Analyzer data channel should comprise of Name, Units, Communication Address, Validity Range, Operation and Error Status. h)Provision to incorporate conversion factors such as PPB to μg/m³ etc.	

Sr. No.	Specifications		Bidder's Response
		 i) Software should be equipped to configure the analysers with it, irrespective of the output mode i.e. Analog or Digital (RS 232) of the instrument. j) System should read raw data values of the analysers and meteorological instruments and duration of averaging data should be user selectable like 10 / 20 / 30 / 40 / 50 / 60 seconds. 	
12)	Data Collection	a) Software should collect each second data. b) Average data over user selectable time	
		 (1, 5, 30, 60 seconds time interval) period. c) Operational status, Error status, calibration status and calibration values observed from the analyzer should be captured and should be made available along with the data with a frequency of maximum five minutes. d) System should collect of the diagnostics of the instrument comprising actual 	
		diagnostics parameters and their values at least once in every five minute to check the state of the health analyzer. e) Calibration parameters i) Provision to entering calibration, span calibration values of gas cylinder/permeation to devices	
Sr. No.	Specifications	.,	Bidder's Response

		further analysis. iii) Provisions to collect electronic system pre calibration & post calibration to ascertain the percentage deviation/ correction	
13)	Data Storage	 a) Data along-with diagnostic, calibration alarms should be stored at station compute at a defined path. b) Interval of data dumping will be same defined in the data collection c) System should be capable to keep ever second acquired data from 32 channels for a period of minimum five years. d) Data stored should be plain text format e) No data encryption should be done at the station and if encryption is done than decryption procedure should be made available in soft file format to check the data at station at any point of time. To convert data on continuous basis for exporting to any other software, if required, procedure should be available 	
14)	Data Display (Statistical analysis of data)	a) In 4-in-4 graphs, 4-in-1 graph and / or 16-in-1 graph formats b) In terms of 4-in-1 table format c) Real time multi - graphs over user selectable time period. d) Display of graphic & tabular display of the current data. e) Graphical form should comprise of 4-4 graphs, 4-1 graphs in user defined format i.e. 1, 5, 10, 15, 30 min, 1hour, 4, 8, 24 hour,	

Sr. No.	Specifications		Bidder's Response
	Specifications	30 days and yearly. (user definable time series) f) Tabular form should comprise of 4 channel list in user defined format i.e. 1, 5, 10, 15, 30 min, 1hour, 4, 8, 24 hour, 30 days and yearly. (user definable time series) g) Station instruments basic configuration etc. should be visible on screen continuously. h) Main window for real time display of all measured parameters with status of all analysers/sensors. i) Statistical analysis tools like regression analysis, co-relation analysis and other analysis as per industry standards in the field of environment should be available and if not the firm should develop these for CPCB within a time frame. j) The system should have procedures for normal analysis tools like calculation of data with respect to a threshold value, average, minimum, maximum, calculation of violating value with respect defined values (Air Quality Standards) for defined period for the database etc. k) Data analysis of diagnostics parameters l) Data analysis of Pre calibration and post calibration data (if facility not available	
		can be developed) m) Data analysis of corrections applied of each calibration cycle (if facility not	

15)	Data Backup	a) There should be defined data backup procedure through which data can be extracted from station computer in simple text format/excel (user definable). b) There should be defined restore procedure also to restore the data in case of data loss. c) A display screen should be available to update the user about data availability.	
16)	Data Validation automatic check at station software	 a) Zero level and span level checks if performed cyclically and defined results are not obtained up to +/- 5% (user definable 0-10%) then system should alarm the user of system failure and the recorded alarm should be transmitted to central software. b) After instruments perform the calibration the results obtained should be recorded and should be transmitted to central computer. 	

4-1			
17)	Data validation requests generated at station computer	At least three tier request generation and request acceptance system procedure is desired. Details are given in the Annexure -I . a) Inbuilt checks capability may be provided, where if instrument throws erratic data software can check automatically and display message and send information in the	
		form of corrected data in corrected database to be approved by the central software at central level. (facility if not available needs to be developed by the system provider) b) There should be provision of two databases one is raw database and another corrected database. (facility if not available needs to be developed by the system provider)	
		c) Validation of data through calibration database Pre calibration & post	

18)	Calibration of systems	 h. Calibration window for analyzer for the calibration from computer. i. Remote Access to Calibration: Calibration exercise need to be done remotely. All necessary arrangements for it should be made in the system. j. Calibration data file may be prepared separately. k. Calibration database need to be formed, stored and transmitted to central. l. Calibration cycles to be as per the models of the instruments. m. Calibration records should store the calibration values displayed by instrument. n. Diagnostics during calibration should also be recorded. 	
19)	Location of station	a) Fixed Station location to be recorded b) Moving station location to be recorded c) Latitude and longitude of stations be recorded	
20)	Data Import	a) In case of communication medium phase there should a mechanism to shift the data into Pen drive (Physical medium for data collection) physically and a procedure to import the same on central software.	

a) Possibility to connect different types printers and auto printing facility for displays generated throughout the

analy

21) Printing

Sr. No.	Specifications		Bidder's Response
		to accept or reject the reasons mentioned by the user end. e) Inbuilt checks capability should be provided, which can be configured by the administrator at central to put alarms according to requirement on data, errors generated or on diagnostics of systems. f) The software at central should have facility to log in data validation requests. These requests will carry the erroneous data for user selected period and for which user at station will request to change the data due to environmental or instrumental operation conditions. These requests will reside in central location and whenever user at central agrees the data will be changed in the validated database. Hence, system will have two types of databases 1) Raw database which can never be touched 2) which has to be modified and corrected as per agreed conditions. The detail of user requesting or applying	
7)	Data Display at Web (if not available facility may be developed by the firm)	 p) System should have standard web display software in place. q) Central software should be capable to show the data in predefined formats at website on a physical map. r) The data from Corrected database shall be displayed on the web. s) Current data should be displayed on web page. 	

Sr. No.	Specifications		Bidder's Response
		t) There should be provisions to show no. of violations occurred, percentage of violation occurred at stations parameters comparing hourly, 8 hourly, 24 hourly and yearly standards u) Provision is required to change standard value, since standard values do change after certain period of time as per Govt. policy. v) Displayed web page should have facility of providing information to all with respect to environment as well as to provide specific files for downloading. w) The logo of CPCB should be displayed on webpage. x) The disclaimer have to be provided on the webpage y) Some predefined queries have to be developed to displaythe data on web page. A search page needs to be developed for converting data into meaningful format for the general public. Help in developing such kind of systems can be taken from existing running system at www.cpcb.gov.in/cpcbpa . z) The current data displayed on the web should have comment inserting facility at individual data and for running data as well like if any station instrument out of order then station official should be able to display message "Instrument under maintenance". aa) Similarly, when data goes beyond a	

Sr. No.	Specifications		Bidder's Response
		defined limit it should automatically display a predefined message as comment on webpage as "Data under Scrutiny". bb) Automatic e-mail messages to be generated for the identified end users to start a corrective action. cc) Station photos to be uploaded for the display along-with the data. dd) User defined 05 pages may be developed additionally, if required by CPCB designs for which may be decided	
10)	Remote Procedures (if not available facility may be developed by the firm)	 h) Central software should have capability to allow to connect any station instrument through remote. i) Central software administrator should be able to go for remote calibration of any of the systems. j) Software should be capable to operate remote stations configurations. k) Control panel window should be available for controlling each analyzer. l) Alarm window for valid alarms of all analysers and sensors. m) It should have transparent data - connection to each analyzer from remote. n) System should be capable to remotely configure all stations through remote location using configuration file to 	

Sr. No.	Specifications		Bidder's Response
		maintain the uniformity. The configuration command from central or from regional location should be active.	
11)	Data Reports Generation	k) To prepare reports hourly, weekly, monthly, yearly in user defined interval and formats. I) Mean, Median, Percentile, Maximum, Standard deviation, Frequency analysis and Maximum Frequency analysis. m)System should have predefined user selectable procedures through which reports of any specific station or multi stations reports upto four parameters can be generated as per user selected time frame. n) Data Comparison Software should be able to compare any of the four channels irrespective of type of data in the system with respect to each other on a single time scale user selectable. o) Data Comparison on different time scale Software should be able to compare data on the basis of different time scales like one station (x) parameter (y) of one given date is compared with other station (z) parameter (y) on any other date in a single graph. p) Data reports, calibration reports and status reports with user time periods. q) Historic multi - curves / graphs over user	

Sr. No.	Specifications		Bidder's Response
		over a period of 1, 15, 30 min, 1 hr, 4, 8, 12, 16 and 24 hrs etc.). s) Diurnal variation, standard deviation, regression and other statistical parameter reporting possibilities with various available mathematical methods. t) If required separate report generation procedures have to be developed for which firm will be responsible for project	
C.	Compatibility	Should have compatibility with the latest Operating System with a contract of 05 (five) years from the date of SUPPLYof software for providing assistance to operate system at CPCB and all the new patches developed for the software during these 05 years without additional cost. Software should have capability of data transmission with the	
D.	Security	c.System should have the facility to have it Password protected or without password as decided by CPCB at the time of implementation. d.System software should be totally secured and any antivirus software required to run the system for the complete project duration has to be managed by the system provider.	
E.	Other Technical Conditions	9. Hardware required for data transmission has to be made available by the firm and there should not be non-compatibility. 10. Firm should have the capability to develop the Software PROTOCOL for	

Sr. No.	Specifications		Bidder's Response
		data transmission from any system available in the field in future during next 05 years or up-to the project period. 11. Should support the latest formats of Windows 32 bit or 64 bit or any other available platform like Linux etc. 12. Manual of complete system should be provided. 13. Firm should provide the hardware required for data acquisition along with all the software's required like OS, MS. Office, Networking software, Remote functionality software, Data uploading software on website, Data display software if required, and should maintain hardware for project duration. 14. Since, system has to be placed in NIC domain for which the web software developed along-with the database and web server software should be certified by CERT-IN empanelled vendors for vulnerability. The system provider is responsible for fulfilling all criteria required to place the system at NIC domain. The firm will be responsible for entire duration of the project for any vulnerability if noticed by NIC. 15. The computers required for the work will be procured by CPCB and configuration for the same will have to be provided by the system provider. 16. Display board will be procured by the	

Sr. No.	Specifications		Bidder's Response
F.	DETAILS OF DESIRED DATA VALIDATION SYSTEM	Annexure-I At least three tier request generation and requests acceptance procedure is desired in the system. It is presumed that level 1 is station, level 2 is Central location at regional level and level 3 at Central level. The regional and central levels will have central station computers and software installed and stations will have station computer installed with station data acquisition software and data transmission software. The flow of data has to be from station to Regional Level and then to Central level. It is desired that environmental database has to be corrected for instrumentation issues as well as for the environmental issues. Hence, officials available at stations will communicate with central and state levels through system itself by commenting on the data. The respective data can be picked up from the database at station itself, corrected to the desired numbers and then transmitted to regional level central computer where, the administrator of system if agrees to the changes desired then data flows to the next level else request is rejected. If request will come to Central server for accepting or rejecting then central level should have authority of accepting or rejecting the data. If central level agrees to the changes than data should be changed in the corrected	

Sr. No.	Specifications		Bidder's Response
		database else request should be rejected. Hence, there should be provisions for accepting or rejecting data at all three levels accordingly. Here, whenever such requests are generated, concerned	
G.	List of protocols for which CAAQM software should support		
	Bayern-Hessen Intercomp5 Inter comp 6 Inter comp 1 Lab Com Metek USA-1 Unor, Oxor AK R+P Defor MBF Multor Gemi Adam Module Uras 14Modbu CLD700 Binos1000 FH62 HP34970A Hygrowin Almemo Gesytec II Modbus RFM433 DGH Module NMEA183 BH/Timo 9600	USA Turbulence Thermo Instr. Thies DL14/15 PR820R Innova1312 PAC3 Multiwarn II Data Collect SDR Meteo Bus VDO Navigation	

H. Checklist to compare Firm's Technical capability table for

specifications of Software

speciti	cations of Software			
S. No.	Details	Capability of firm's software as on date	Firm agrees or disagree to develop software in future	If firm agrees to develop application then time frame from individual activity
1.	Data transfer interval Max. 5 minutes from all locations?			
2.	System will transmit data along with diagnostics. If yes then how many channels diagnostics values shall be transmitted to central and at what duration?			
3.	System will transmit data along with Calibration values (Pre cal and Post Cal)?			
4.	System has remote calibration procedures in place for Regional level and central level both?			
5.	System has remote configuration facility for regional and central level both?			
6.	System has database validation procedure in place?			
7.	Web software already developed or not?			
8.	If Web software is available is it modifiable as per CPCB need by the firm?			
9.	Whether agree to develop five web pages as per mutual discussion			
10.	Web software with password and or without password			
11.	Password providing facility available at regional levels			
12.	Statistical tools available at web software or not?			
13.	System provider is capable of placing system in NIC domain			
14.	System provider will provide certification from CERT-IN empanelled firms			
15.	Data import from other files			
16.	Data export to other files			
17.	Pre defined queries to be inbuilt for providing data to public whether these are already available or to be developed if yes then time frame?			
18.	Standards comparison and exceedances be reported on web			
19.	Different types of predefined formats of report preparation available or not?			
	SUPPLY INSTALLATION AND COMMISSIONING AND	ODEDATION & MAI	NTENANCE SERVICE	-C OF



20.	ssupport various protocols available till		
	date as listed provided or not?		
21.	If new protocol based software is to be		
	developed whether firm will		
22.	Unlimited Number of stations supported		
	by Central Server software or not? If not		
	then support for how many stations will		
	be provided		
23.	System compatibility with		
	Dialup/BB/2G/3G/Wireless available or		
	not? If not then what technologies		
	supported as on date? What time		
	frame if other to be develop.		
24.	Software has Wind rose reports		
	generating capability		
25.	Software has pollution rose generating		
	facility		
26.	Software has diurnal variation facility		
27.	Software has mathematical tools		
28.	Software has 16 channels display at on		
	page		
29.	Software has data communication error		
	reports		
30.	System has error correction procedure		
31.	Software has parallel data display		
	reports		
32.	Software has virtual channel		
	deployment capacity		
33.	Software has data encrypting		
	procedures at stations or not? If yes		
	then data can be retrieved from station		
	or not?		
34.	Software compatible for ANDROID		
25	technology		
35.	System Provider will provide all		
	Hardware required at station and Central		
26			
36.	System Provider all necessary software		
	required for data acquisition, display,		
	Analysis, website uploading etc.		



DISCLAIMER

1.1 Though adequate care has been taken in the preparation of this E Bidding Document, the Bidder should satisfy himself that the Document is complete in all respects. Intimation of discrepancy, if any shall be informed in pre-bid meeting on prior submission as per the tender condition. If this office receives no intimation by the date mentioned in this document, it shall be deemed that the Bidder is satisfied that the Bidding Document is complete in all respects.

Member Secretary
Maharashtra Pollution Control Board
Kalpataru Point, 3rd floor,
Opp. Cine Planet Cinema, Sion Circle
Sion (E), MUMBAI – 22
Ph: 022-24014701

Fax: 022-24024068

- 1.2 Neither MPCB, nor their employees or consultants make any representation or warranty as to the accuracy, reliability or completeness of the information in this RFP nor is it possible for MPCB to consider the financial situation and particular needs of each party who reads or uses this Document. MPCB recognizes the fact that certain prospective Bidders may have a better knowledge of the Project than others and thus encourages all prospective Bidders to conduct their own investigations and analysis and check the accuracy, reliability and completeness of the information in this Document and obtain independent advice from appropriate sources.
- 1.3 Neither MPCB nor their employees or consultants will have any liability to any prospective Bidder or any other person under the law of contract, tort, the principles of restitution or unjust enrichment or otherwise for any loss, expense or damage which may arise from or be incurred or suffered in connection with anything contained in this RFP, any matter deemed to form part of this Document, the award of the Project, the information and any other information supplied by or on behalf of MPCB or their employees, any consultants or otherwise arising in any way from the selection process for the Project.
- 1.4 **MPCB** reserves the right to reject any or all of the Bids submitted in response to this *E Bid Document* atany stage without assigning any reasons whatsoever.
- 1.5 **MPCB** reserves the right to change any or all of the provisions of this *E Bid Document*. Such changes would be intimated to all parties procuring this *Document*.